


WILD M695

Operating microscope

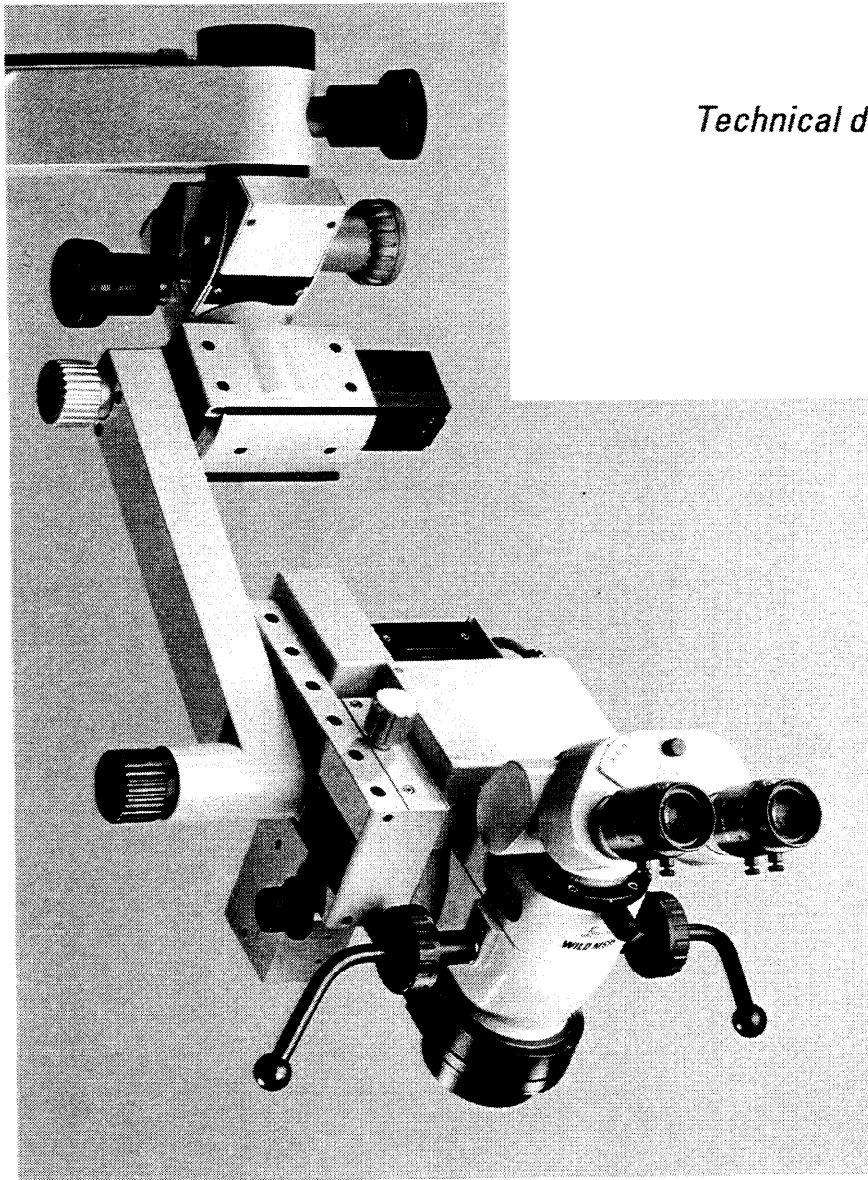

Service manual *Technical description and fault finding*

*Doc Code 636 718
Edition 09/93*

*Revisions
10/94*

Copyright by Leica AG, Heerbrugg, Switzerland 1994

Leica AG, CH-9435 Heerbrugg (Switzerland)
Telephone +41 (071) 70 31 31, Fax +41 (071) 72 69 52
Leica is a registered trade mark of Leica technologij B. V. Rijswijk, the Netherlands

Leica

Service Manual

WILD M695

Operating microscope

Legal matters	1
Revisions/Service News	2
Introduction / User manual	3
Fault finding with testset	4
Control unit MEL61/62, MEL64/65	5
Swingarm MSV 136/137	6
Microscope M695	7
	8
Wiring diagram	9
Replacing modules	10
Replacing boards	11
Inspection procedure	12
	13
	14
	15
	16
Training	17
Testset	18
Spare parts catalogue	19
Special tools	20

Leica

Inhaltsverzeichnis / Table of contents

Kapitel	Seite
Rechtsfragen / Legal questions	1
Sicherheit / Safety / Securite / Seguridad	3

Rechtsfragen / Legal questions

Copyright

Ohne vorherige schriftliche Erlaubnis der Firma Leica AG, Heerbrugg (Schweiz), darf dieses Dokument weder insgesamt noch auszugsweise mit mechanischen, fotografischen, elektronischen oder irgendwelchen anderen Mitteln (einschließlich ihrer Umwandlung oder Übertragung in maschinenlesbarer Form) kopiert, in einem Informationsspeicher abgelegt, außerhalb des dafür vorgesehenen Zwecks oder in irgend einer Form an von Leica AG, Heerbrugg nicht ausdrücklich befugte Dritte zugänglich gemacht oder abgegeben werden.

Haftung

Dieses Dokument richtet sich ausschließlich an qualifizierte Servicetechniker und Servicetechnikerinnen, welche über die notwendigen Fachkenntnisse verfügen.

Qualifizierte Servicetechniker und Servicetechnikerinnen sind solche, die den entsprechenden Servicekurs bei Leica AG, Heerbrugg erfolgreich besucht haben und bei Unternehmen der Leica Gruppe oder bei von Leica AG, Heerbrugg autorisierten Vertretungen oder Servicewerkstätten tätig sind.

Wird dieses Dokument von nicht qualifizierten Servicetechniker und Servicetechnikerinnen verwendet, so lehnt Leica AG, Heerbrugg jegliche Haftung ab für direkte und indirekte Schäden, die durch nicht fachgemäße Anwendung und/oder Interpretation dieses Dokumentes entstehen.

Copyright

Without prior permission in writing by Leica AG, Heerbrugg (Switzerland), this document shall not be reproduced as a whole or in part, by mechanical, photographic, electronic, or other means (including into or transmission in machine-readable form); stored in any retrieval system; used for any purpose other than that/those for which it is intended; nor made accessible or communicated in any form to any third party not expressly authorized by Leica AG, Heerbrugg to have access thereto.

Liability

This document is strictly for the use of qualified service engineers with the requisite technical skills.

Only persons who have successfully completed the appropriate service training provided by Leica AG, Heerbrugg and are in the employ of a Company in the Leica Group or of an agency, distributor, or Service Workshop duly authorized by Leica AG, Heerbrugg have the status of qualified Service engineer.

Leica AG, Heerbrugg accepts no liability whatever for direct or indirect damage that may occur due to the unauthorized or improper use or interpretation of this document by any person who is not a qualified service engineer in accordance with the above definition.

Sicherheit / Safety / Sécurité / Seguridad

Für die Servicetechniker und Servicetechnikerinnen gelten folgende Pflichten:

- Sie verstehen und befolgen die Sicherheitsinformationen und die Instruktionen auf dem Produkt sowie in der Gebrauchsanleitung.
- Sie kennen die ortsüblichen gesetzlichen, betrieblichen und ausserbetrieblichen Unfallverhütungsvorschriften im Wissen, dass sich diese auf dem aktuellsten Stand befinden.
- Sie benachrichtigen Leica schriftlich, sobald an der Ausrüstung Sicherheitsmangel auftreten.

Service technicians have the following obligations:

- To understand and follow the safety information and instructions on the product and in the user manual.
- To be familiar with local regulations relating to industrial and non-industrial accident prevention in the knowledge that these regulations are up to date.
- To inform Leica immediately in writing if the equipment becomes unsafe.

REVISION

Documentation : **WILD M695 Service manual**
(Technical description and fault finding)

Status : Edition 09(93) / Revision, previous: -----
new: 10/94


Reason for revision : M680 control unit (MEL61/62) is compatible with M695

Steps to be taken :

Section	Remove page(s)	Number of sheets	Introduce page(s)	Number of sheets
---	title sheet	1	title sheet	1
---	index register	1	index register	1
2	---	--	2-1/2	1
9	9-1 to 9-8	4	9-1 to 9-8	4
19	19-1	1	19-1	1

File : Insert this sheet (Revision) in section 2.

Leica AG
 Service Documentation
 and Training LSG/SOM/SM

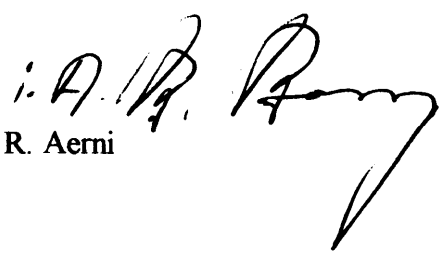
 R. Aerni

No. 10/95

To Service staff

Leica AG
CH-9435 Heerbrugg
(Switzerland)

Date/from June 28, 1995 / 3077-HWE

File Workshop binder "Service News" / Service manual M695

Re. **M695 surgical microscope in conjunction with multifocus objective 445 944**

Multifocus objective on M695: Readjustment of the illumination

Restriction of illuminated area

When the multifocus objective is used with the M695, the illuminated area available to the surgeon may be shadowed or vignetted even when the the lamp is correctly adjusted.

Inspect the illumination

When you use the multifocus objective for the first time, inspect the illumination:


- Engage the shortest working distance (the shortest focal length).
- Engage the lowest zoom position (7).
- Inspect the illuminated fields produced by **both** of the lamps in the lamp changer.
- If the illuminated area is noticeably restricted, readjust the lamps.

Readjusting the lamp

The illumination of the field of view is influenced by the distance between the lamp and the condenser lens. This distance can be changed by means of the eccentric stop cam on the lamp changer. To obtain uniform illumination, reduce the distance between the lamp and the condenser lens.

Adjust the eccentric stop cam for both lamps in the lamp changer:

1. Remove the multifocus objective and push the filter slide of the M695 optics carrier towards the objective. Beneath the filter slide you will find the adjusting screw for the eccentric stop cam.

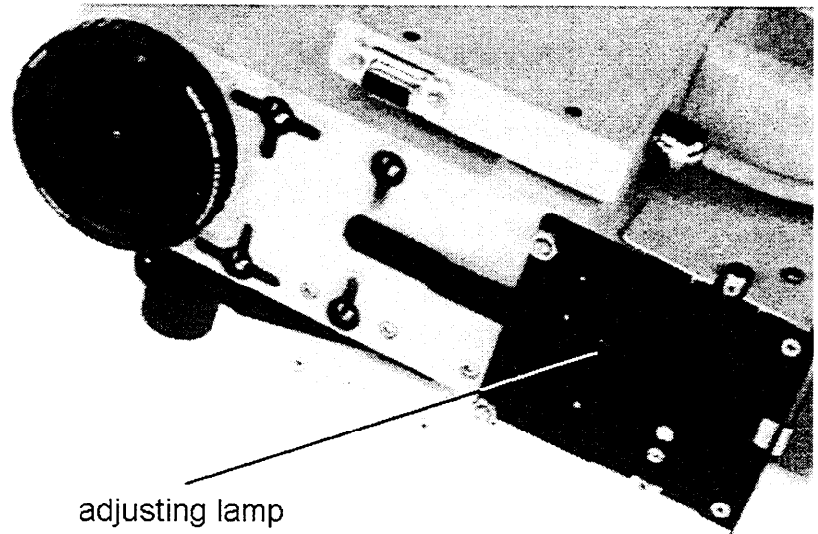


adjusting lamp

2. Using a screwdriver, displace the eccentric stop cam by about one-eighth of a turn so that the lamp can be moved in the direction of the objective.


CAUTION: The lamp may be hot.

3. Switch to the second lamp, and carry out point 2 for this lamp.
4. Refit the multifocus objective and inspect the illumination as described above.
5. If necessary, repeat the adjustment procedure (points 1 - 3).

Leica AG
Service SOM/SM



K. Bieniek



W. Hammerle

No. 09 / 95

To Service staff

Leica AG
CH-9435 Heerbrugg
(Switzerland)

Date/from May 29, 1995 / BKL-3402

File Workshop binder "Service News" / Service Manual M695

Refer to **Necessary replacement of SOM product "Light intensifier"**
No. 445 796

Faulty product has to be exchanged

Delivery of faulty SOM product "Light intensifier" 445 796

The concerned product has been delivered to the following countries as single part or included in the delivery of optics carriers:

Netherlands, Japan UK, Italy, Australia, USA, Sweden, Canada, Switzerland, Korea, South Africa, Kuwait, Belgium, Spain Columbia, Saudi Arabia, France, Singapore, Finland, Portugal, Germany, Denmark, Algeria, Sudan, Luxembourg, Dominikanische Republic, Hong Kong, Turkey, Brazil, Tunisia, Israel, Austria, Jordanian India.

All other countries are not concerned.

Problem:

Since market introduction in March 1994 up to March 1995 the concerned product has been delivered faulty (The cement does not withstand the high temperatures at the bulb). It has been delivered as a single part as well as included in the following optics carriers:

M690 optics carrier Mitaka 445 543

M695 optics carrier 445 560

M695 optics carrier Mitaka OH 445 841

Since March 1995 an improved version with the same No. has been delivering. The two versions can be distinguished easily according to the drawing on page two.

Action:

The concerned customers are already informed by your Management.

The faulty products have to be replaced, please contact your Marketing responsible for SOM products.

All concerned countries will be supplied automatically without any order with sufficient replacement units, free of charge.

The exchange procedure is very simple and can be achieved by the customer himself as well. If you will not carry out the exchange yourself, supply the customer with sufficient exchange units and Information.

The action of replacement has to be achieved ASAP and should be finished by end of September '95 at the latest.

Please send a **feedback after fully finish of the action of exchange** with a list of all concerned customers to the

SOM HOTLINE: Fax: ++41 - 71 - 72 26 77


This is necessary for reasons of product liability.

Your expenses on this action will be refunded by us via the 'Repair Report to Factory' (Please fill out the report completely, one report for the complete action!).

Fig.1:


The improved (second) version has

approx. 5 mm cement free area in the center,

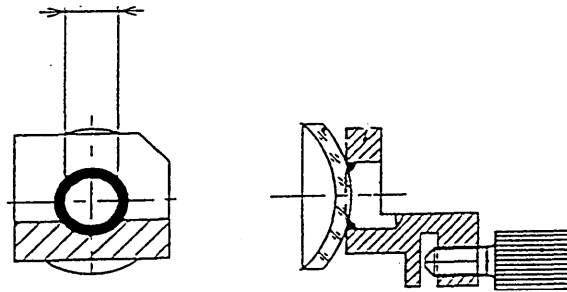

good improved version

where at the old version the whole is completely filled with cement.

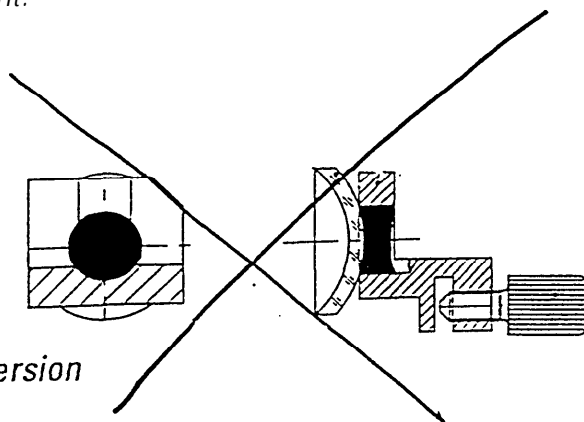

old version

Leica AG
Service SOM/SM

Klaus Bieniek

Klaus Bieniek

Werner Hämmerle
Werner Hämmerle

Changes and modifications

M680 control unit (MEL61/62) is compatible with M695 surgical microscope

**... from control unit
serial number 011193001
onwards**

the MEL61/62 can also be used for the M695, provided that earlier lamp control PCBs are subjected to a slight modification. This modification was introduced from March 1993 onwards (Index C on board) (355 980 C).

The functions ZOOM SPEED B, XY-SPEED and POSITION 1/2 are not required for the M695. The positions occupied on the control panel by these switches or potentiometers will be covered over. The covers, and instructions for fitting them, accompany the control unit.

From March 1995 onwards, only the MEL61/62 control unit will be used for the M680 and M695. The previously-used MEL64/65 control unit will no longer be manufactured.

Modification of the lamp-control PCB


is required if both of the following conditions are met:

1. The MEL64/65 control unit is replaced by an MEL61/62
2. The M695 was despatched before March 1993. The lamp control PCB therefore bears an earlier index than C.

Under these conditions the hand-/footswitches will not react at the control input A or B respectively, depending on the position of the switch "Position 1/2".

Modification: On the soldered side, bridge pins 10 and 12 of P20 with a 100 Ω resistor (1/8W). The resistor shall not come into contact with the housing cover.

LAMP CONTROL BOARD

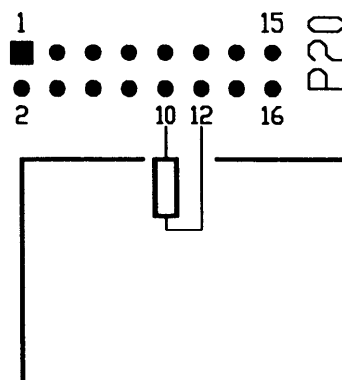

Preconditions for using this service manual

Intended users

Technical personnel provided by customer or by LEICA agencies, equipped with the testset 566 152 (see Section 18).

What is expected of the person using the Testset?

Stage 1: Allocation of a fault to one of the main groups:

- ***Footswitch***
- ***Control unit***
- ***Swingarm***
- ***Microscope (optics carrier)***

- You have read the user manual and can operate the surgical microscope

Directions are given in Sections 3 and 4.

Stage 2: Locating and eliminating errors at module level

- You have been trained in the basics of electronics and mechanical engineering
- You have been instructed by a technician from your agency or from LEICA AG, HEERBRUGG.

Sections 3,4 and 10

Stage 3: Locating and eliminating errors at board level

- You have been trained in the basics of electronics and mechanical engineering
- You have taken part in an M690/M695- or M680 course.

Sections 3 to 9, and Section 11

To the contents of service manual

Legal aspects

This book may only be given to, and used by, certain persons. These are detailed in **Section 1**.

Changes/ Service News

Place Service News on top of the M695 in **Section 2**.

Introduction/ User manual

CONGRATULATIONS - You are one of those methodical people who also read the important **Section 3** of this manual.

locating faults with the test set (Test box)

If a fault develops, **we will** guide you **to** it with **the** assistance of **Section 4** and the test box.

The test set helps you to assign the fault to the:

- Footswitch
- Control unit
- Swingarm
- Microscope

The search is then continued at board level with the assistance of block diagrams and the wiring diagram.

Control unit MEL64165 Description of function

The function description in **Section 5**, in conjunction with the wiring diagram, will lead you to the defective board or cable connection. The swingarm is the interface.

Swingarm

Description of function

The function description in Section 6, in conjunction with the wiring diagram, will lead you to the defective board or cable connection. The swingarm is the interface.

M680 microscope

Description of function

The function description in **Section 7**, in conjunction with the wiring diagram, will lead you to the defective board or cable connection. The swingarm is the interface.

Wiring diagram

Section 9 contains the wiring diagram, and a description of the positions of the boards and the plug connections.

Exchanging modules

Section 10 includes instructions for exchanging those modules which are available as spare parts.

Exchanging boards

Section 11 includes instructions for exchanging those boards which are available as spare parts.

Testing procedure

After modules or boards have been replaced, the instrument must meet specifications. Values and tolerances are laid down in the testing procedure **in Section 12**.

Test set

The test box and service cable, and their circuits, are described in **Section 18**.

Spare parts

The spare parts, the exchange of which is described in Sections 8 and 9, are listed in **Section 19**.

Special tools

Section 20 includes a list of the service equipment which will enable you to carry out the operations described above.

No special tools are required. The components making up the test box include a service handswitch and a service cable which serves to bridge the swingann.

***The M695 User Manual is provided as a separate document.
To view it, click on this text.***

Table of content

M695 fault finding


Chapter	Page
Preparation	4-1
Power supply of control unit	4-3
Functions of hand- or footswitch	4-4
Supply of microscope	4-5
Lamp control	4-7
Zoom control	4-8
Focus control	4-9

M695 Fault finding

Preparation


1. Connecting the testbox

- Disconnect plug P36 from swingarm
- Hook in the testbox to the swingarm and plug in P36 at the testbox.
- Connect the testbox cable (green sleeve) with J36 at the swingarm. With that the control unit is connected with the microscope through the testbox.
- Set switch "MICROSCOPE SELECT" on the testbox to position A.

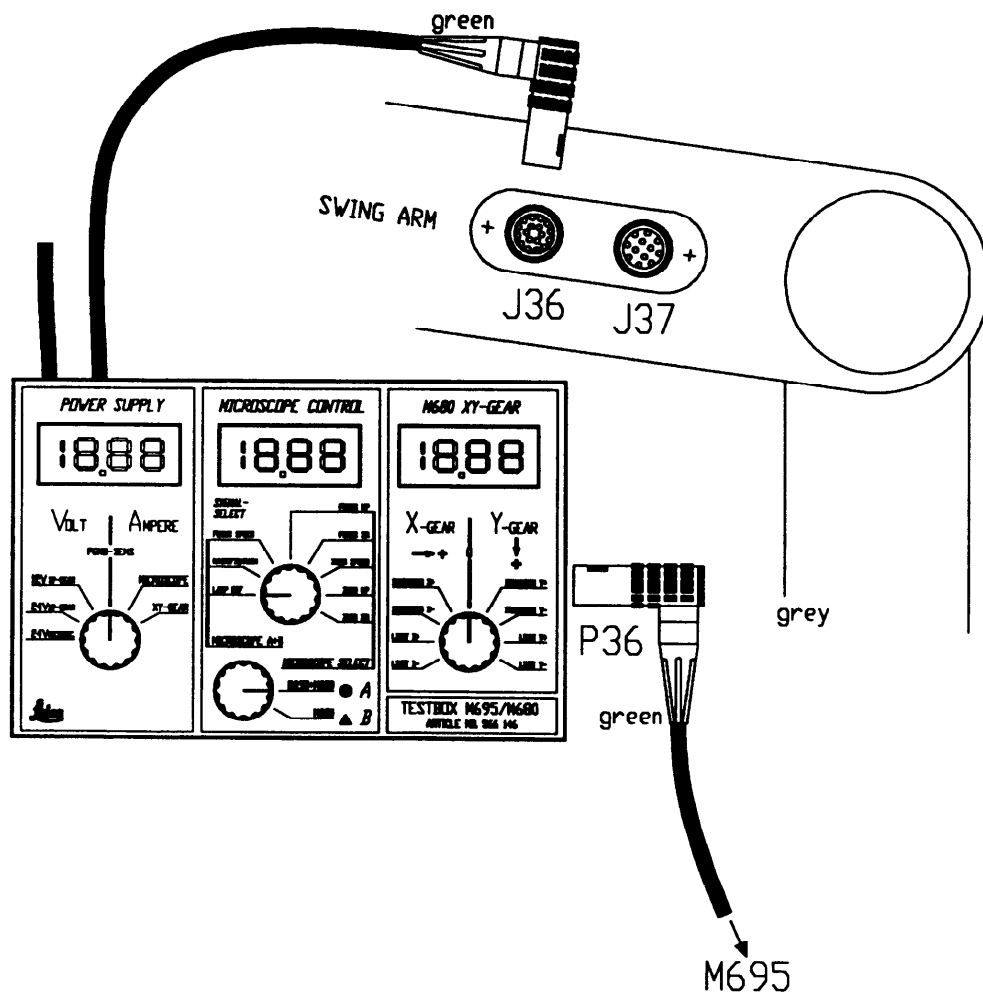

2. Settings on the control unit

- Adjust Lamp to minimal brightness

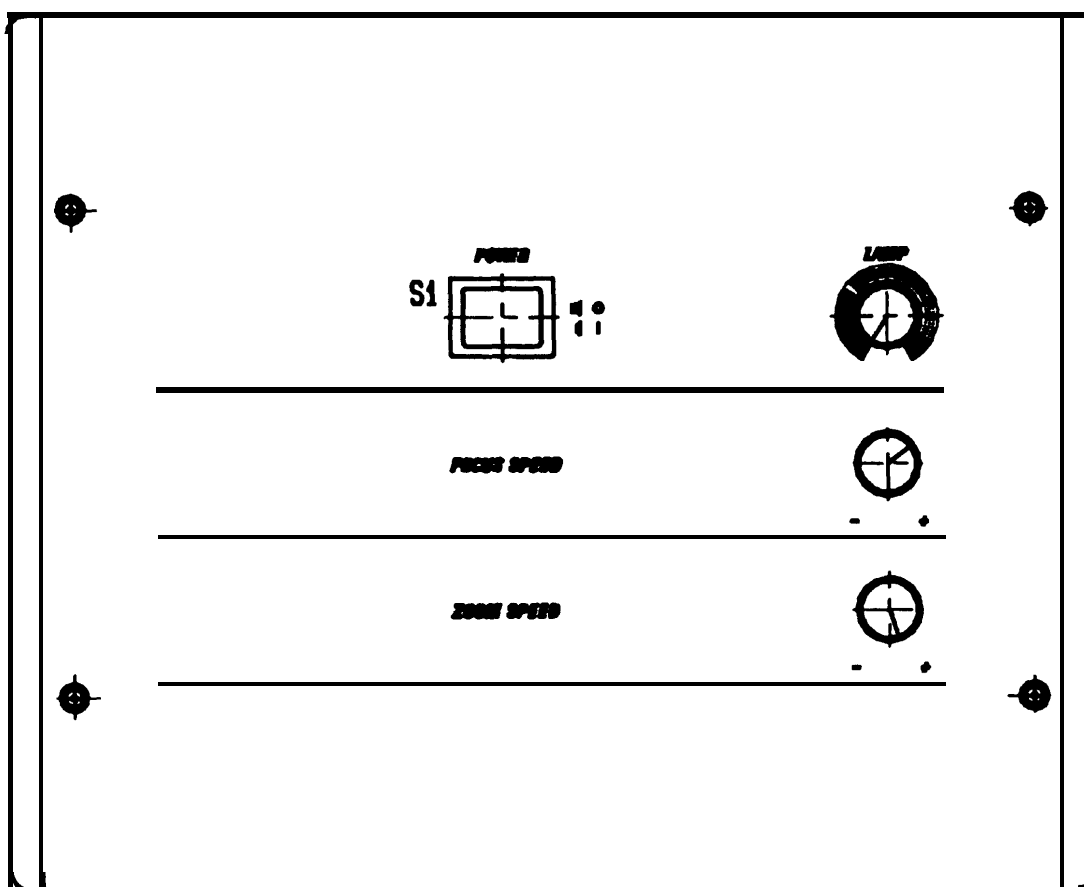


Power supply of control unit

<i>Action</i>	<i>Reaction</i>	<i>Possible reason</i>	<i>Check</i>
SWITCHING ON	Lamp of main switch does not light	Line voltage	Fuses F1 and F2 in line plug P1 Main switch S1 Line cable
	5V-LED on Function-Display does not light	24V-main supply	Transformer Rectifier circuit Wiring
		10V-supply	Panel board
5V-supply		Receiver board	
	Focus does not move to center position	Control unit, Swingarm or microscope	Focus control page 4-9


Functions of hand- or footswitch

Condition: Malfunction of hand- or footswitch of only one of the two CONTROL-inputs, A or B
is disturbed.


- **Replace disturbed hand- or footswitch ective side A or B** by either:
 - a) Service-handswitch or
 - b) Hand-/footswitch at the other CONTROL-input

<i>Action</i>	<i>Reaction</i>	<i>Possible reason</i>
<p><i>Release functions:</i></p> <p> SL→ (F) Z↑ Z↓ F↑ F↓ </p> 	<p>Corresponding LED at Function Display does not light</p>	<p>Receiver Board</p>
<p><i>Connect again original switch and release functions</i></p>	<p>Corresponding LED at Function Display does not light</p>	<p>Hand- or footswitch</p>

Supply of microscope

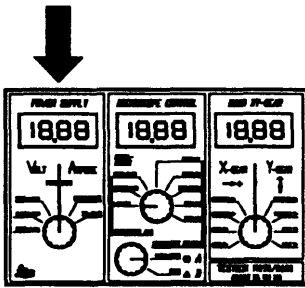


Voltage	Action	Reading	Reaction	Possible fault
24V <small>MICRO</small>	1.Lamp to min.brightness 2.Lamp to max.brightness 3.Lamp back to min. brightness	26V +5% 20V +5%	Microscope reacts - but incorrect	Check supply- lines of 24V and check PGND - page 4-6
			Microscope without any function	Wiring of microscope
	Switch off, bridge swing- arm with servicecable and switch on again	26V +5%	microscope reacts	Swingarm cable
Switch off, Separate microscope from testbox and switch on	26V +5%	Voltage ok		evtl. short circuit in the microscope
			Voltage not ok	Control unit

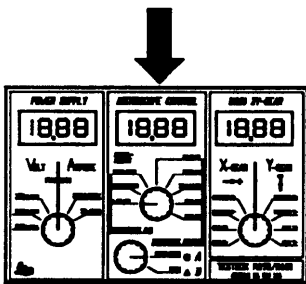

Check lines of Powerground PGND
(Voltage drop on PGND relating to logic ground)


Signal	Action	Reading	Reaction	Possible fault
FOCUS UP	Adjust lamp to maximal brightness	max. -0.8W with standard-swingarm cable	If voltage is ok - depending on the incorrect function, check signals of: Lamp control - page 4-7 Zoom control - page 4-8 Focus control - page 4-9	
	Bridge swingarm with service cable and adjust lamp to max. brightness	max. -0.8V	Voltage ok	Swingarm cable (One of the two PGND-lines is broken)
			Voltage not ok typ. >-1v	One of the two PGND-lines in the microscope or control unit is broken.
Important: Adjust lamp again to minimal brightness!				

Lamp control

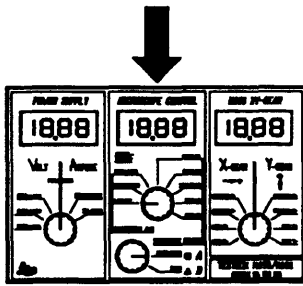

Signal	Action	Reading	Reaction	Possible fault
LAMP REF	Adjust lamp to min./max brightness	0.3V / 5V +-5%	Voltage ok	Microscope (Lamp Control, Wiring)
	Separate microscope from the testbox, adjust lamp to min./max brightness	0.3V / 5V +-5%	Voltage ok	Microscope
	Bridge swingarm with service cable, adjust lamp to min./max brightness	0.3V / 5V +-5%	Voltage ok	Swingarm cable
			Voltage not ok	Control unit
Important: Adjust lamp again to minimal brightness!				

Focus control

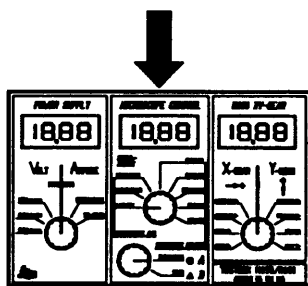

Select microscope side A or B:

- Select A or B, depending on which side the zoom works incorrect
- Select A if the fault appears on both sides, A and B.

Signal	Action	Reading	Reaction	Possible fault
FOCUS SPEED	set min. focus speed set max. focus speed	1.25 ... 1.27V 5v +-5%	Voltage ok, but reacts incorrect	Microscope (Focus servo, wiring)
FOCUS UP	Release F↑ on hand-/footswitch non-actuated	>4.75V <0.2V		
FOCUS DN	Release F↓ on hand-/footswitch non-actuated	>4.75V <0.2V		
	Separate microscope from the testbox and check signals	see above		
	Bridge swingarm with servicecable and verify signals	see above	Voltages ok	Swingarm-cable
			Voltages not ok	Control unit

Table of content

Description of functions MEL64/65 control unit

Chapter	Page
Introduction	5-1
Power supply	5-3
Lamp control	5-9
Zoom control	5-11
Focus control	5-15

Description of functions MEL64/65 control unit

The description is subdivided for the main groups:

- Control unit MEL64/65 - Section 5
- Swingarm MSV136/137 - Section 6
- M695 microscope - Section 7

The control circuits for zoom, focusing and XY-gear

are located partly in the control unit and partly in the microscope itself. Their functions are described in the following sections 5 and 7.

The swingarm cable

is the electrical link between the control unit and the microscope, and is therefore the ideal place to start looking for faults at the level of the main groups.




The test box is introduced between the swingarm and the microscope. It can be used to study the supply voltages, control signals and control levels, all of which are transmitted through the swingarm cable. Section 6 includes a list of these signals.

Notes

Power supply MEL64/65



Tasks	Control elements /displays	Pages
24V supply for microscope and XY-gear	Red LED on panel board indicates defective fuse	5-6
10V supply for potentiometer and receiver board	Green LED on panel board shows 10V O K	5-6
5V supply for logics of receiver board and footswitch or handswitch	LED "5V" OK on function display	5-7
Ground		
PGND: Microscope ground	Yellow LED on panel board indicates switch-off caused by excess current	5-7
SENS	Logics (ground) microscope	5-7
GND_XY: XY ground		

PANEL BOARD

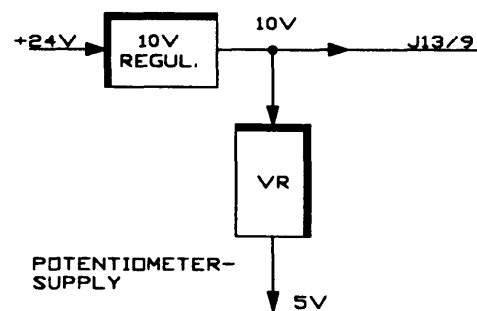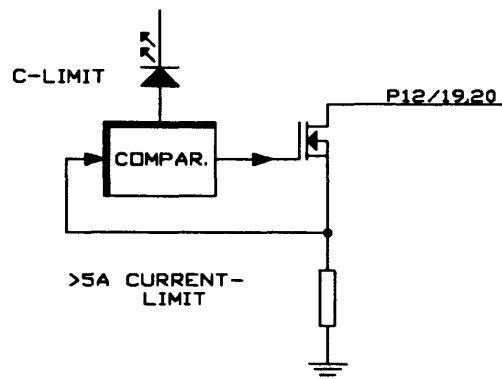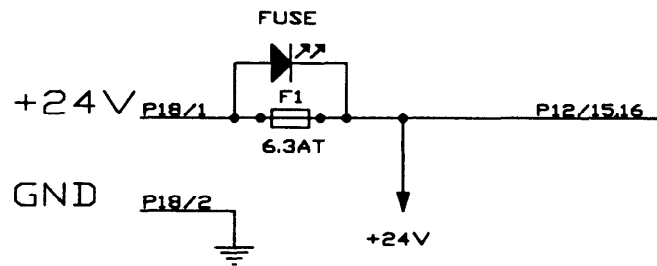

RECEIVER BOARD

SWING ARM

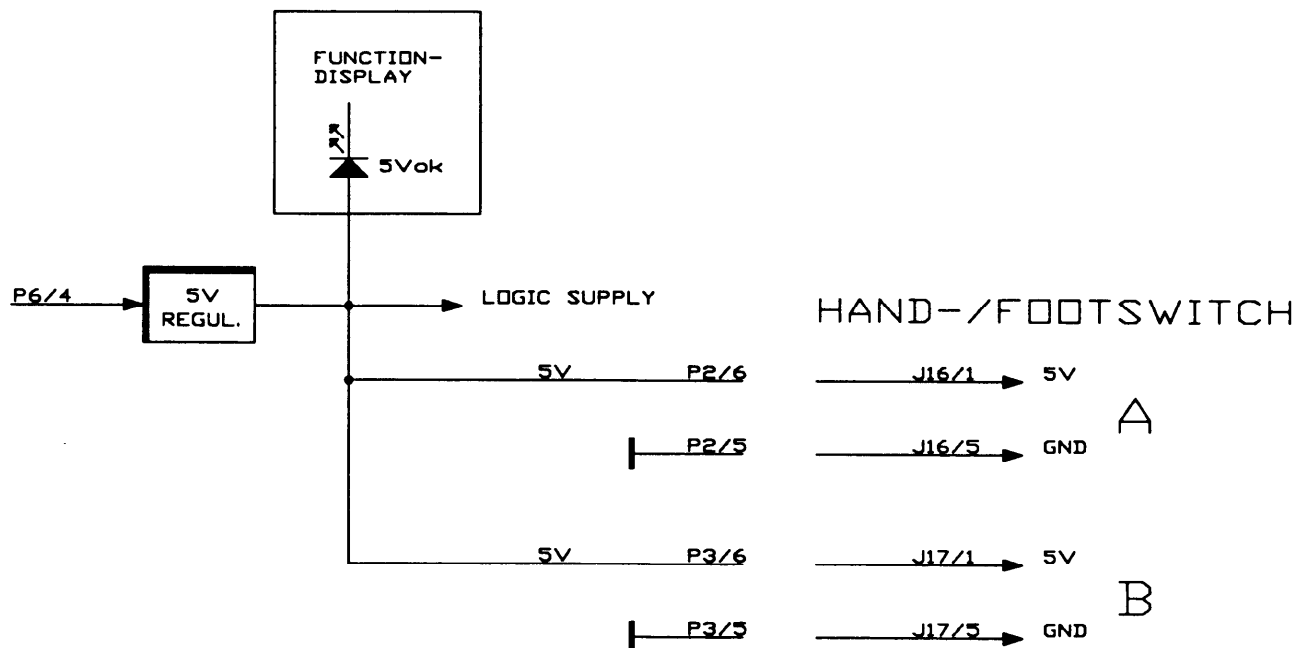

Control-LEDs

On the panel board:

10V OK: green LED shines

>5A on 24V (PGND): yellow LED shines

Fuse interrupted: red LED shines

and on the function display:

5V OK: green LED shines

24V supply

The 24V supply powers the servo board via the receiver board, and the microscope via the swingann.

The fuse for the unstabilized main supply voltage is on the panel board (6.3AT). The red LED indicates a burnt fuse.

Limitation of excess current

The loading at maximum lamp **brightness** is about 3.25A. The yellow LED on the panel board indicates switching off as a result of excess current (5A) at PGND.

10V supply

A switching regulator on the panel board reduces the 24V to 10V. The power for the potentiometer (5V) is derived from it. The 5V regulator on the RECEIVER BOARD is supplied with 10V.

5V supply
Receiver board

An LED on the function display shows 5V OK. The following are supplied with power: Handswitch or f&switch, and logics on receiver board.

PGND, SENS and logics
ground

Microscope ground (PGND) and SENS are connected in the microscope. The high lamp current produces a voltage drop of about 0.6V at PGND. This voltage is passed to the control unit through SENS.

For the reason indicated above, Logic ground is about 0.6V below PGND in the microscope. The voltage drop at PGND influences the level of the control signals.


SENS

All control signals to the microscope are measured with the testbox in relation to SENS. SENS is connected to GND trough a 20-Ohm resistance at panel board.

Notes

Lamp control MEL64/65

<i>Tasks</i>	<i>Control element/display</i>	<i>Pages</i>
<i>Setting the lamp brightness</i>	Potentiometer on control unit	5-10,7-3
<i>Limiting excess current</i>	Measurement resistor on LAMP CONTROL in microscope	7-3

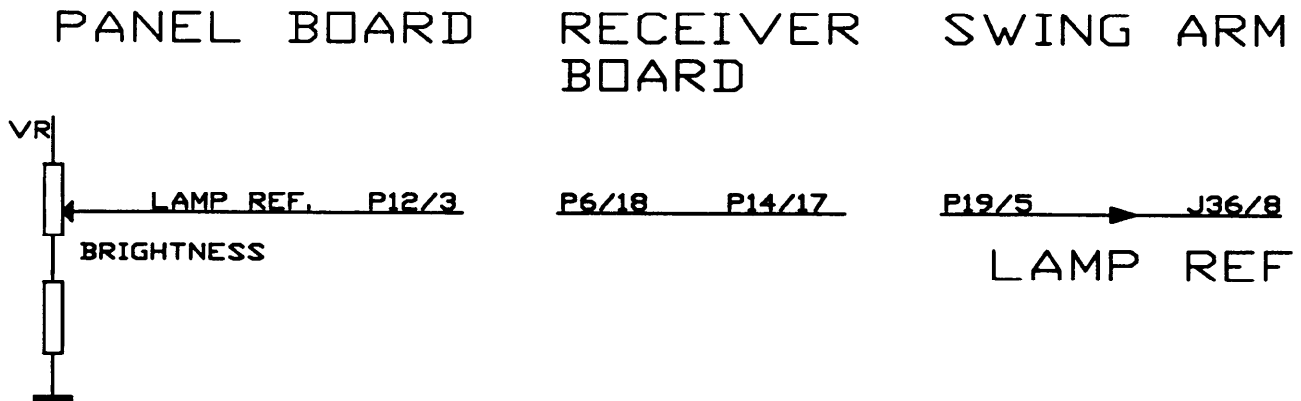

Reference for lamp regulator



The voltage level LAMP REF depends on the position of the brightness potentiometer. LAMP REF is passed via the receiver board and the swingarm cable to the lamp control board in the microscope, where it forms the reference value (required value) of the lamp regulator.

	<i>LAMP REFerence</i>
<i>Min. brightness</i>	0.3V +5%
<i>Max. brightness</i>	5.0V +5%

Zoom control MEL64/65

Tasks	Control elements / display	Page
<i>Using motor to set zoom position</i>	Footswitch or handswitch Function display Up/down-LED on zoom servo	5-14,7-6
<i>Presenting zoom adjustment speed</i>	Zoom speed potentiometer	5-14,7-8

PANEL BOARD

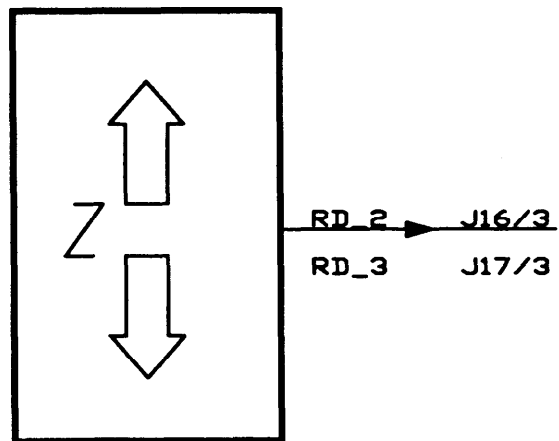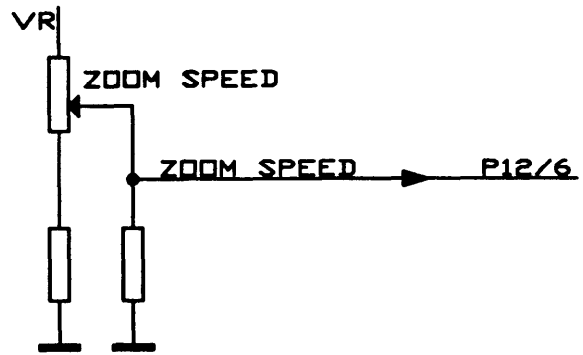

Control LEDs

The function display tells you whether the signals from the footswitch or handswitch are being correctly received and interpreted:

Z↑ for ZOOM UP
Z↓ for ZOOM DOWN

Using the motor to set the zoom position

The handswitch or the footswitch transmits on RD_2 or RD_3 the codes which correspond to the functions:

Data format:

ASCII 8-bit with start bit
repeating at 2.3-millisecond intervals
+5W/-8V

The logics on the receiver board (processor) assign the codes received to their appropriate functions:

ZOOM UP
ZOOM DOWN

The control signals (0V/5V) for ZOOM UP and ZOOM DOWN reach the logics board in the microscope via the swingarm cable.

Presetting the zoom displacement speed



The voltage level of ZOOM SPEED depends on the position of the potentiometer on the panel board.

	<i>Level of ZOOM SPEED</i>
<i>min. ZOOM SPEED</i>	$2.10V \pm 0.25V$
<i>max. ZOOM SPEED</i>	$5V \pm 5\%$

Focus control MEL 64/65


<i>Tasks</i>	<i>Control elements/display</i>	<i>Pages</i>
<i>Motorized focusing</i>	Footswitch or handswitch Functiondisplay Up/down-LED on focus servo	5-18,7-
<i>Presetting speed of focusing</i>	Focus speed potentiometer	5-18,7-
<i>Travelling to centre position</i> after switching on or resetting	Footswitch or handswitch Reset switch on motor driven objectiv (MOBxxx)	5-19,7-

PANEL BOARD

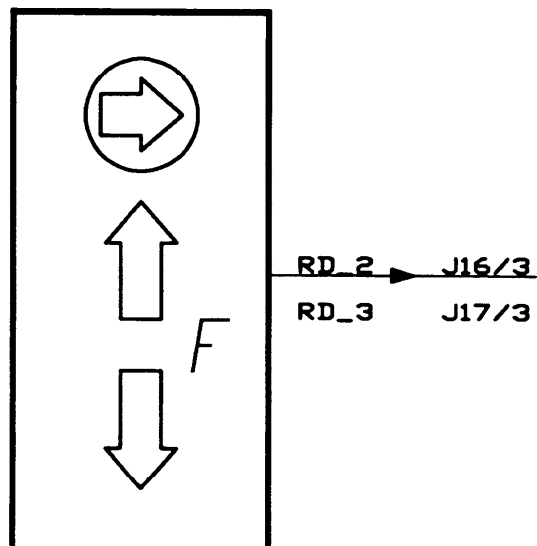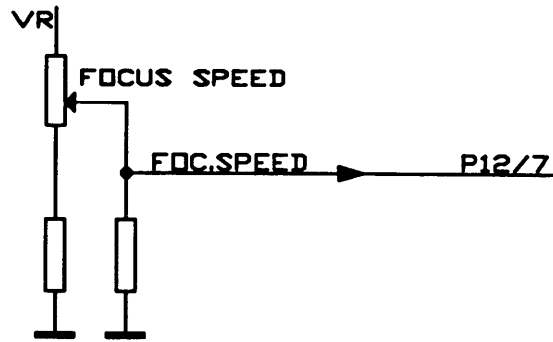

RECEIVER BOARD

SWING ARM

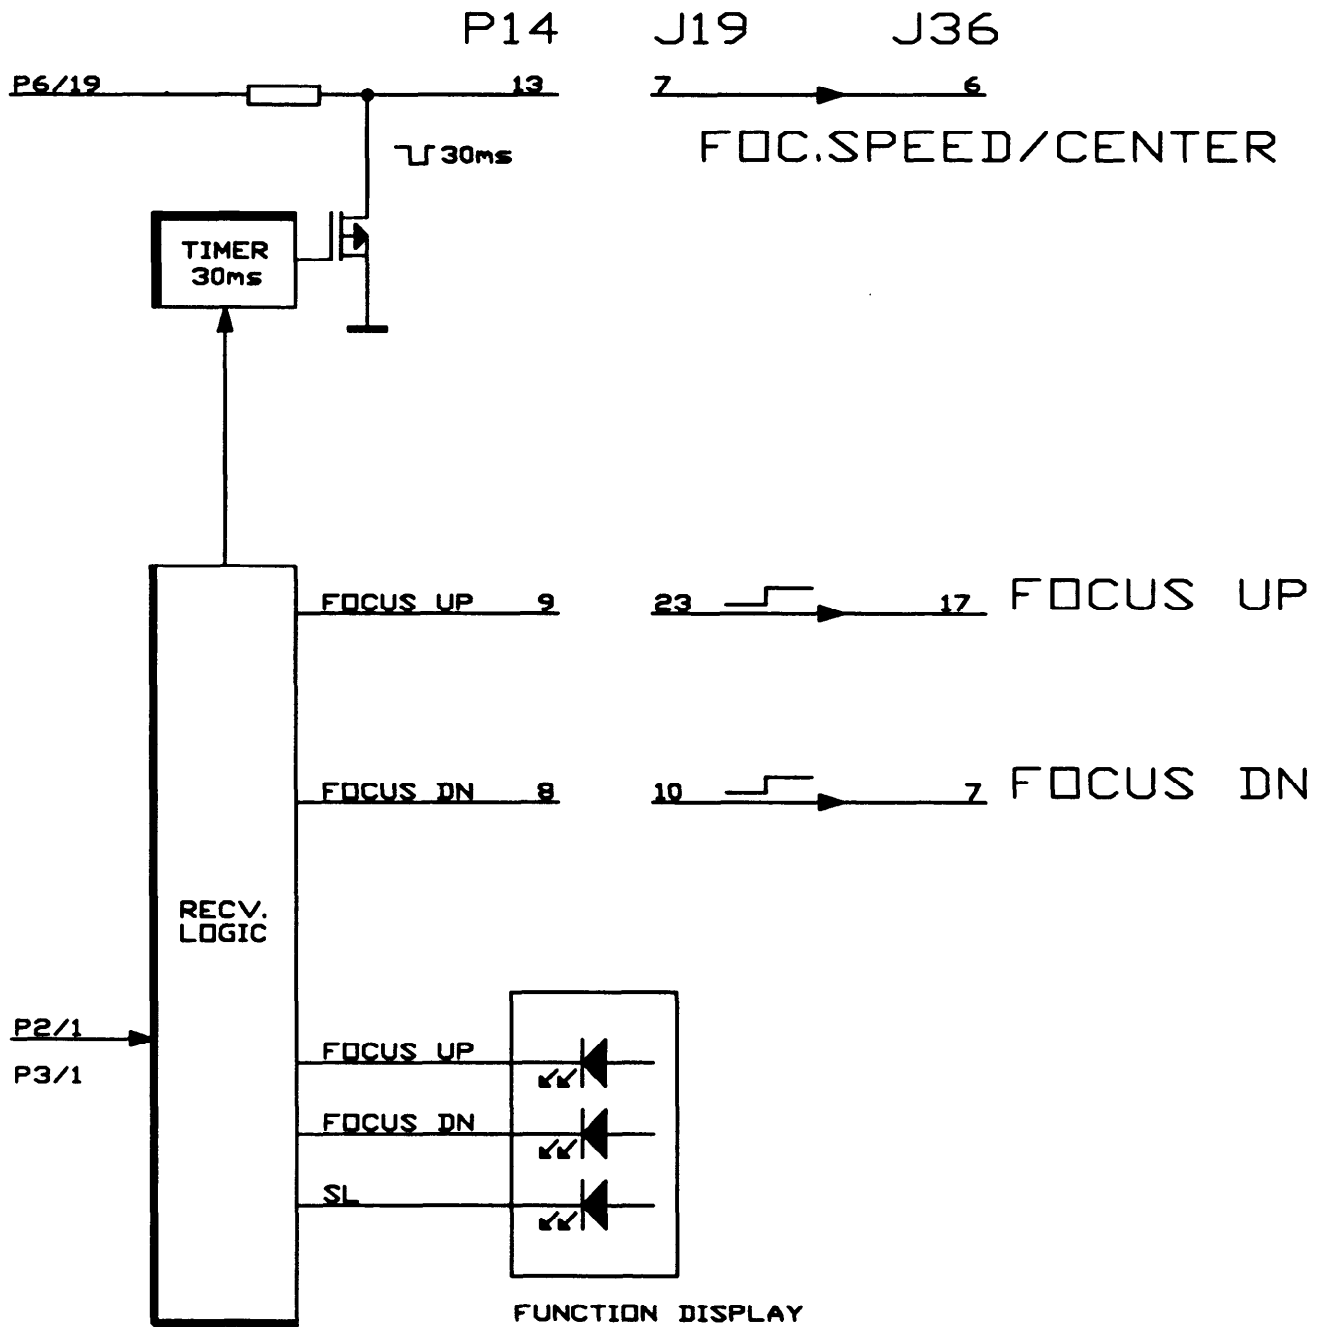

Control LEDs

The function display tells you whether the signals from the footswitch or handswitch are being correctly received and interpreted:

F↑ for FOCUS UP
F↓ for FOCUS DOWN
SL→ for CENTER POSITION

Motorized focusing

The handswitch or footswitch transmits on RD_2 or RD_3 the codes which correspond to the functions:

Data format:

ASCII 8-bit with start bit
repeating at 2.3-millisecond intervals
+5V/-8V

The logics on the receiver board (processor) assign the received codes to their appropriate functions:

FOCUS UP
FOCUS DOWN
CENTER POSITION

The control signals (0V/5V) for FOCUS UP and FOCUS DOWN reach the logics board in the microscope via the swingarm cable.

Presetting the focusing displacement speed

The voltage level of FOCUS SPEED depends on the setting of the potentiometer on the panel board.

	<i>min. FOCUS SPEED</i>	<i>max. FOCUS SPEED</i>
<i>Zoom position 25</i>	0.5V-0.7V	2.1V +5%
<i>Zoom position <8</i>	1.25V-1.7V	5V +5%

Travelling to mid-position

This function is activated from the handswitches or footswitches A and B, using the key (SL->). A timer (Monoflop) sets FOCUS SPEED to GND potential for about 30 milliseconds, using a transistor.

The impulse is recognized on the focus servo in the motor driven objective (MOBxxx), and the system is steered to the mid-position.

Notes

Table of content

List of signals for swingarm MSV136/137

Chapter	Page
Power supply	6-1
Microscope control	6-3

List of signals for swingarm MSV 136/137

Required values for standard two-metre swingarm cable

- Unless otherwise indicated, set the lamp to minimum brightness, because the values quoted are only valid under these conditions.

Power supply

SIGNAL	CONDITIONS	VALUE	TOL.
24VMICROSCOPE	Voltage against PGND Lamp min. brightness ->	26V	+5%
	Voltage against PGND Lamp max. brightness ->	20V	+5%
PGND	Voltage against SENSE Lamp min. brightness ->	-50mV	
	Voltage against SENSE Lamp max. brightness ->	-250mV	
	Voltage drop against logics level Lamp min. brightness: -> (Test box: Microscope Setting: Focus up)	4.9V	-0.2v
	Voltage drop against logics level Lamp max. brightness -> (Test box: Microscope Setting: Focus up)	4.2V	-0.8V

Current consumption Microscope	Lamp min. brightness →	150mA
	Quick-change lamp mount disengaged →	50mA
	Lamp max. brightness Guiding value →	3.5A

Microscope control

All signals are measured against SENSE

Unless otherwise indicated, set the lamp to minimum brightness

<i>SIGNAL</i>	<i>CONDITIONS</i>	<i>VALUE</i>	<i>TOL.</i>
LAMP REF	Lamp min./max. brightness	0.3...5V	+5%
FOCUS SPEED	Min./Max.	1.25...1.7V / 5V	+5%
FOCUS UP	Low/High	<0.2V / >4.75V	
FOCUS DN	Low/High	<0.2V / >4.75V	
ZOOM SPEED	min./max.	1.84...2.34V / 5V	+5%
ZOOM UP	Low/High	<0.2V / >4.75V	
B ZOOM DN	Low/High	<0.2V / >4.75V	

Table of content

Description of functions M695 microscope


Chapter	Page
Power supply	7-1
Lamp control	7-3
Zoom control	7-5
Focus control	7-9

Power Supply

M695 microscope

For functions of control unit, refer to page 5-3

<i>Tasks</i>	<i>Page</i>
24V-Supply	7-2
Ground PGND, SENS	7-2

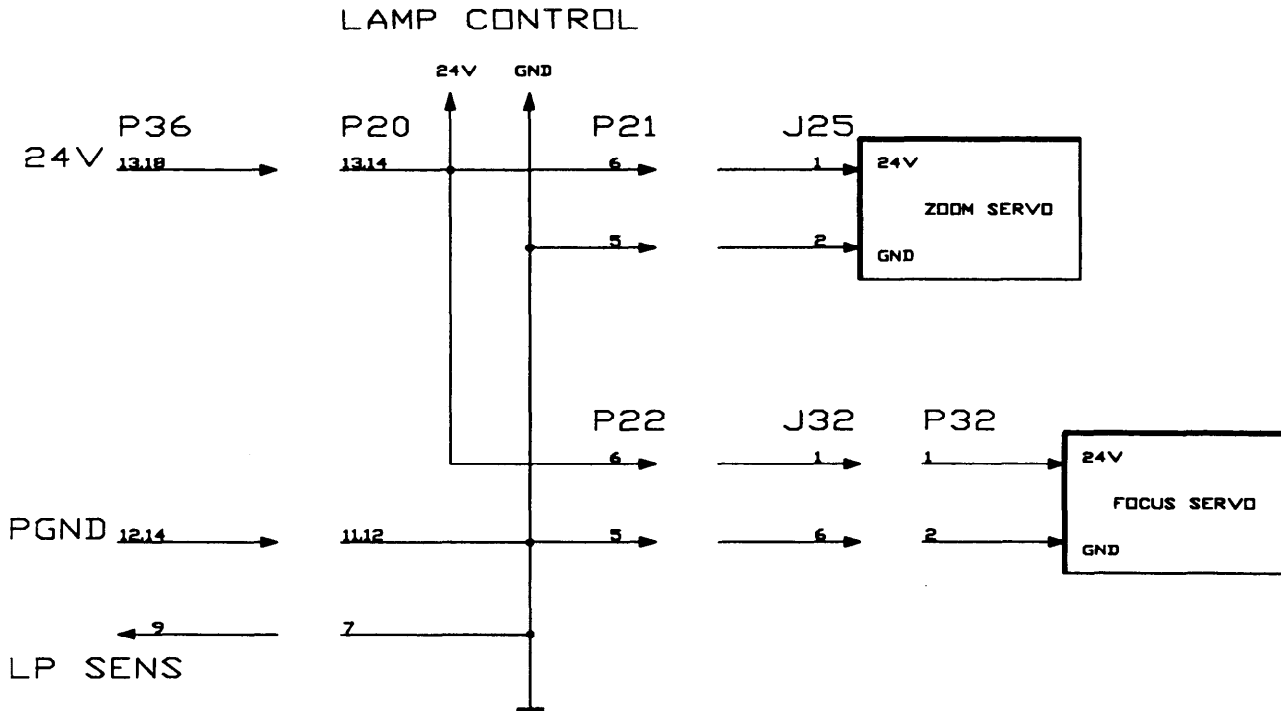

24V supply

**Lamp Control
Zoom Servos A+B
Focus Servos A+B and**

The final stages for lamp, zoom- and focusing motor, is supplied with 24V on these boards, via switching regulators.

PGND, SENS and Logics-Ground

Microscope-Ground (PGND) and SENS are linked within the microscope. The high lamp current causes a voltage drop of about 0.6V to PGND. This voltage is passed to the control unit through SENS.

Situation up until July 1993 ...

For the reason indicated above, Logics-Ground is about 0.6V below PGND in the microscope. The voltage drop at PGND affects the level of the control signals, and so longer swingarm cables than the standard ones can result in malfunctioning.

New situation as from August 1993

Logics-Ground in the control unit is connected to SENSE and so is partly dependent on PGND. The effect on the control signals is therefore less and longer swingarm cables can be used.


Lamp control

M695 microscope

For functions of control unit, refer to page 5-9

<i>Tasks</i>	<i>Control elements / displays</i>	<i>Page</i>
<i>Setting the lamp brightness</i>	Control unit	7-4
<i>Limiting the excess current</i>	Measuring resistor on LAMP CONTROL	7-4

LOGIC BOARD

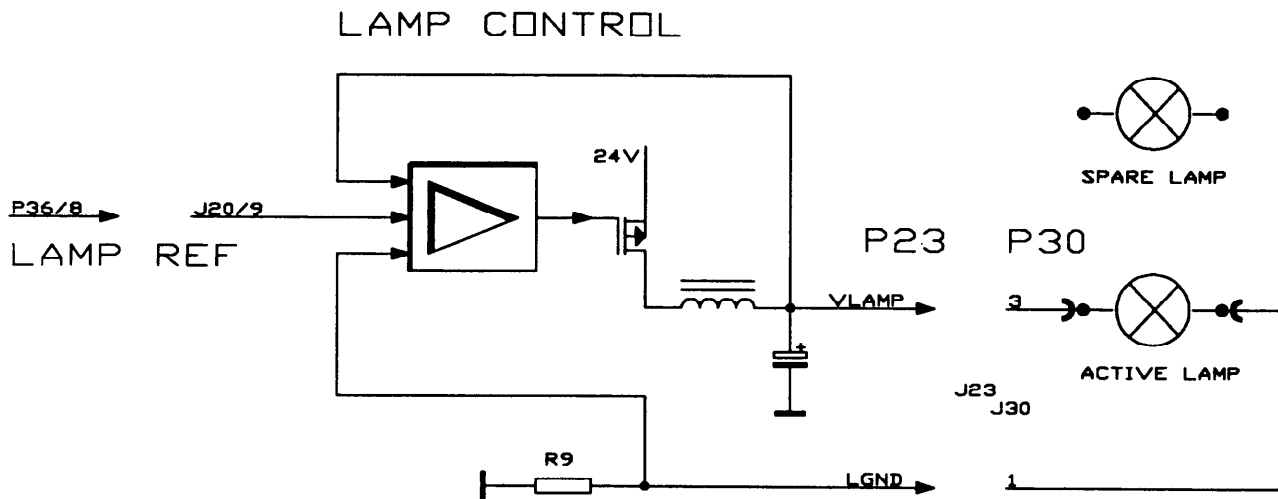

Adjusting the lamp brightness

A pulse-width modulator, dependent on the level of LAMP REF, controls the final-stage transistors. The voltage is smoothed with chokes and electrolytic condensers and the electricity is conducted to the lamp.

The secondary voltage is compared with the required value (LAMP REF) at the entrance of the regulator.

Limiting the excess current

The lamp current produces a voltage drop across resistor R9 in Lamp-Ground (LGND). The regulator measures this voltage drop and limits the current to 5A during the final stage.




Zoom control

M695 microscope

For functions of control unit, refer to page 5-11

<i>Tasks</i>	<i>Control elements /displays</i>	<i>Page</i>
<i>Setting zoom position with motor</i>	LEDs: ZOOM UP + DOWN	7-6
<i>Recognizing end of range</i>	Light barriers on ZOOM SERVO	7-7
<i>Presetting zoom displacement speed</i>	Control unit	7-8

LAMP CONTROL

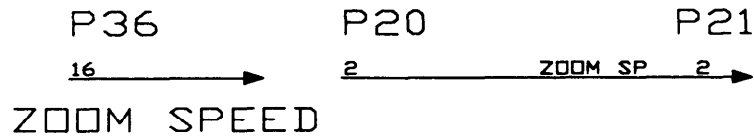

Control LEDs


Yellow LEDs on the zoom servo board for the signals

ZOOM UP

ZOOM DOWN

Using motor to set zoom position...

The control signals (0V/5V) for ZOOM UP and DOWN reach the zoom board via the swingarm cable and lamp control board in the microscope. ZOOM UP/DOWN activates the final-stage transistors on the zoom servo board. The end-stage comprises a bridging circuit of transistors. In accordance with the direction of displacement the transistors are activated by two: T1 and T3, or T2 and T4.

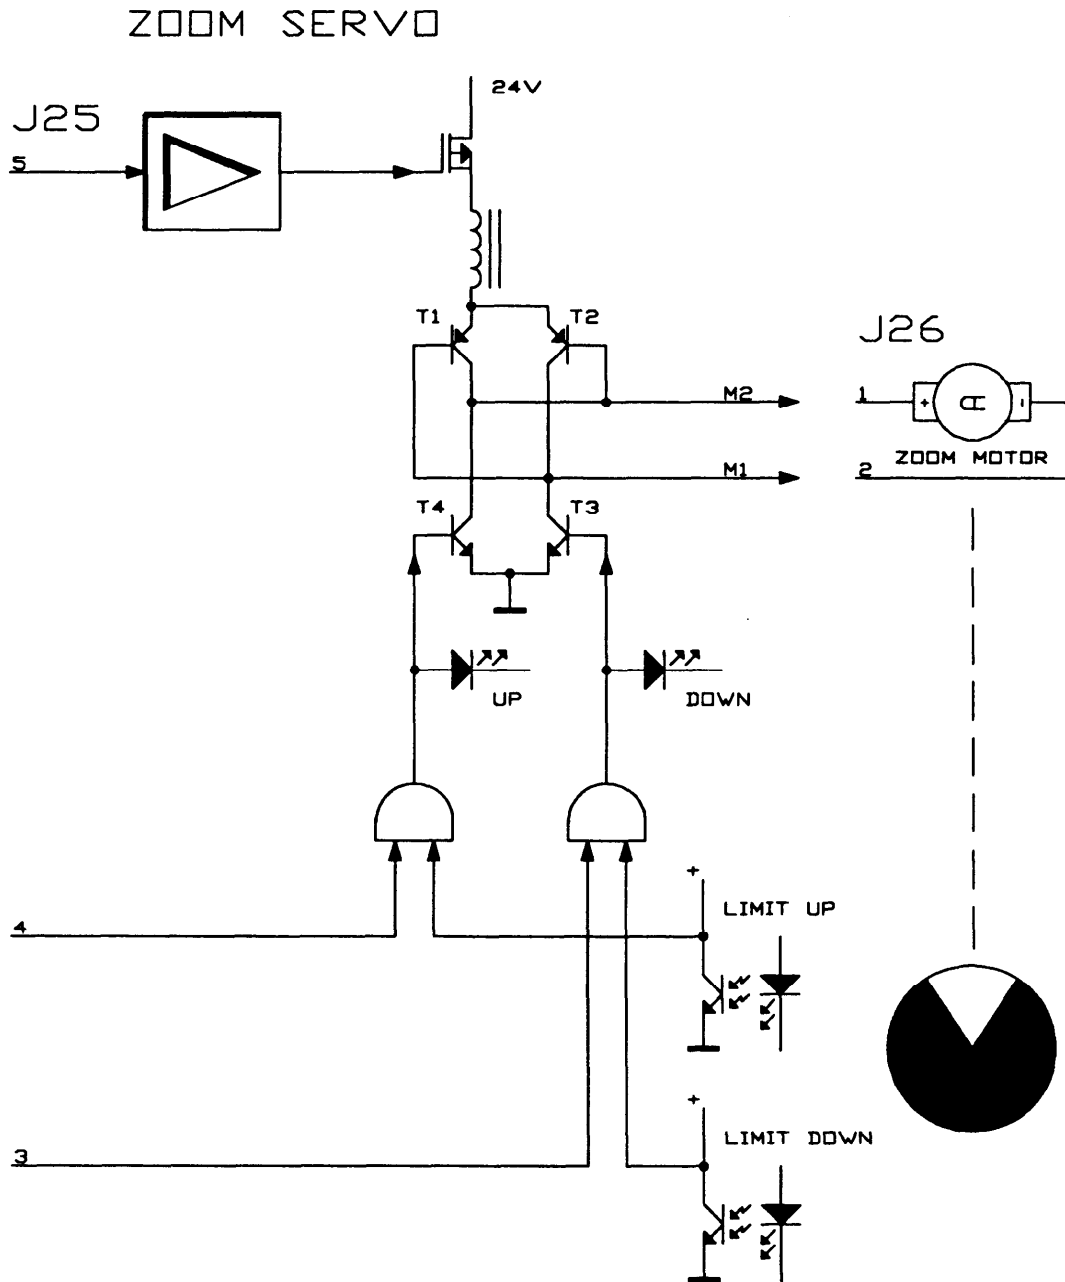

Recognizing end of range

An encoder disk rotates with the zoom gear. The white field on the disk is marking the limit area. It is sensed by two light barriers located on the zoom servo.

If one of both light barriers senses the white field, through a gate the transistor bridge is blocked for that direction of displacement.

Before removing the encoder disk: Mark the disks position at its flange. The adjustment of the disk is described in section 11 - "Replacing boards" (Zoom servo).

***Presetting the zoom
displacement speed***

The displacement speed is adjusted by means of the supply voltage for the zoom motor. The final stage only has a switching function. The ZOOM SPEED level is the reference for the voltage regulator on the zoom servo board.

The regulator has a positive current feedback, and so the motor voltage increases with the load. The current through the final stage is limited to about 150mA.



Focus control

M695 microscope


For functions of control unit, refer to page 5-15

<i>Tasks</i>	<i>Control elements /displays</i>	<i>Page</i>
<i>Motorized focusing</i>	Control unit	7-12
<i>Recognizing end of range</i>	Light barriers on FOCUS SERVO	7-12
<i>Presetting the focus displacement speed</i>	Control unit	7-12
<i>Travelling to the mid-point</i>	Focus reset switch Control unit	7-12

LAMP CONTROL

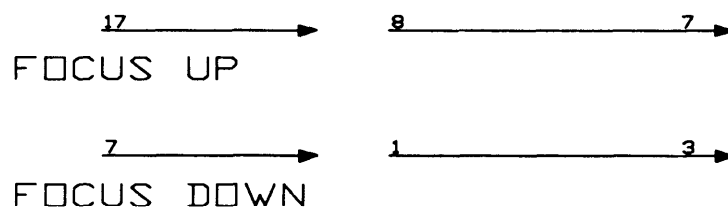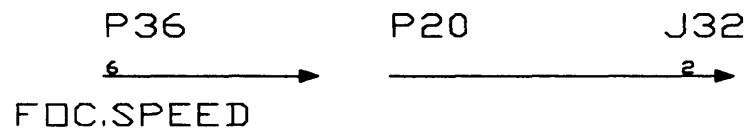

FOCUS SERVO

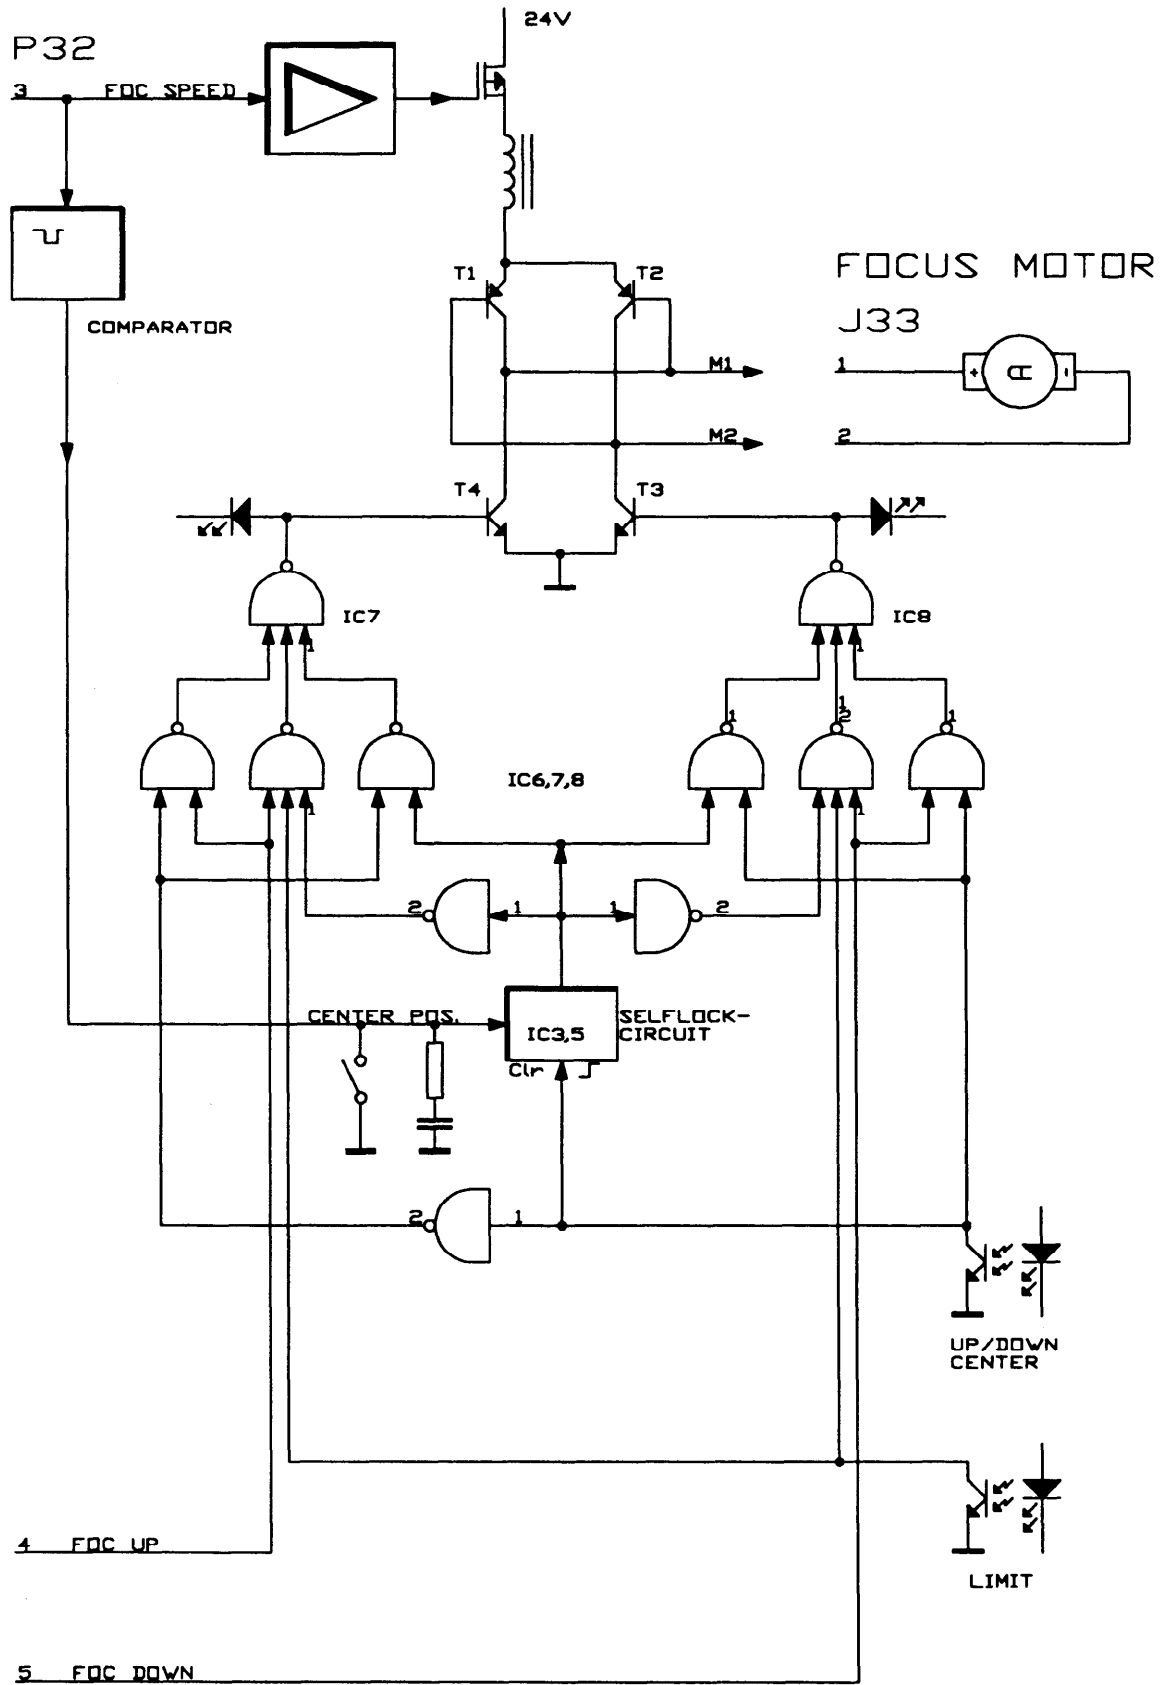

Motorized focusing

The control signals (0V/5V) for A/B FOCUS UP and A/B FOCUS DOWN pass through the swingarm cable and the Lamp Servo to reach Zoom Servo at the microscope. ZOOM UP/DOWN activates the end-stage transistors in the zoom servo board. The end-stage consists of a bridging circuit of transistors, and so the motor can drive the focusing mechanism in both senses of rotation.

Recognizing end of range

Reflexive light barriers sense 2 encoder tracks at the circumference of the focus gear: UP/DOWN+CENTER and LIMIT.

With the light barrier UP/DOWN, through gate 2 or 5, the direction of the arrived limit position is decoded. Through gate 2 or 5 LIMIT blocks FOCUS UP or DOWN at the following NAND-gate. The final stage is then blocked for that direction.

Presetting the focus displacement speed

The displacement speed is altered with the supply voltage for the focus motors. The final stage only has a switching function. The FOCUS SPEED level is the reference for the voltage regulator on the focus servo board.

The current through the final stage is limited to about 140mA.

Travelling to the mid-position

Triggered by:

- Pressing key "Center Position" at the focusing unit
- Switching on the microscope.
- 30ms-pulse to FOCUS SPEED from control unit. The comparator recognizes when FOCUS SPEED is at GND potential.

The following functions are activated as a result:

1. The selflock circuit is triggered. Gate 2 and 5 block FOCUS UP and DOWN to the final stage. The voltage supply for the focusing motor is switched to maximal speed.
2. Lightbarrier UP/DOWN+CENTER senses, at which side from mid-position the focus gear is staying. Through gate 3 or 4 the final stage is controlled - the motor drives the focus gear toward mid-position...
3. ...until the light barrier on the sensor board detects the crossing from dark to bright at mid-position. The selflock circuit is reset (Clr) - the motor stops.

Referenz auf Steckverbinder **Reference to connectors**

Wo im Instrument die Steckverbindungen zu finden sind erfahren Sie anhand dieser Liste und der nachfolgenden Seiten.

The location of connectors is shown by the list, referring to following pages.

Steckverb. Connector	Seite Page	Einheit Unit
P1	9-4,9-5,9-6	Steuergerät - Control unit MEL64/65
JP2	9-6	Steuergerät - Control unit MEL64/65
JP3	9-6	Steuergerät - Control unit MEL64/65
JP6	9-6	Steuergerät - Control unit MEL64/65
JP7	9-6	Steuergerät - Control unit MEL64/65
JP8	9-6	Steuergerät - Control unit MEL64/65
JP9	9-6	Steuergerät - Control unit MEL64/65
JP12	9-7	Steuergerät - Control unit MEL64/65
JP14	9-6	Steuergerät - Control unit MEL64/65
J16	9-4,9-5,9-6	Steuergerät - Control unit MEL64/65
J17	9-4,9-5,9-6	Steuergerät - Control unit MEL64/65
JP18	9-7	Steuergerät - Control unit MEL64/65
J19	9-4,9-5,9-6	Steuergerät - Control unit MEL64/65
P19	9-8	Schwenkarm - Swingarm MSV 136/137
JP20	9-10	Mikroskop - Microscope M695
JP21	9-10	Mikroskop - Microscope M695
JP22	9-10	Mikroskop - Microscope M695

Steckverb. Connector	Seite Page	Einheit Unit
JP23	9-10	Mikroskop - Microscope M695
JP25	9-11	Mikroskop - Microscope M695
JP26	9-11	Mikroskop - Microscope M695
J27	9-4,9-5,9-6	Steuergerät - Control unit MEL64/65
JP30	9-11	Mikroskop - Microscope M695
J32	9-12	Mikroskop - Microscope M695
P32	9-10	Mikroskop - Microscope M695
JP33	9-12	Mikroskop - Microscope M695
J36	9-9	Schwenkarm - Swingarm MSV136/137
P36	9-10	Mikroskop - Microscope M695
J37	9-9	Schwenkarm - Swingarm MSV136/137



Referenz auf Boards **Reference to boards**

Boards finden Sie anhand der Liste und der nachfolgenden Abbildungen.



The location of boards is shown by the list, referring to following pages.

Board	Seite Page	Einheit Unit
Focus Servo	9-12	Mikroskop - Microscope M695
Function Display	9-6	Steuergerät - Control unit MEL61/62, MEL64/65
Lamp Control	9-10	Mikroskop - Microscope M695
Panel Board	9-7	Steuergerät - Control unit MEL61/62, MEL64/65
Receiver Board	9-6	Steuergerät - Control unit MEL61/62, MEL64/65
Zoom Servo	9-11	Mikroskop - Microscope M695
XY Servo Board	9-6	Steuergerät MEL61/62 - Control unit MEL61/62 keine Funktion im M695 - no function with M695


Steuergerät MEL61/62 - Anschlussplatte
Control unit MEL61/62 - Connector panel

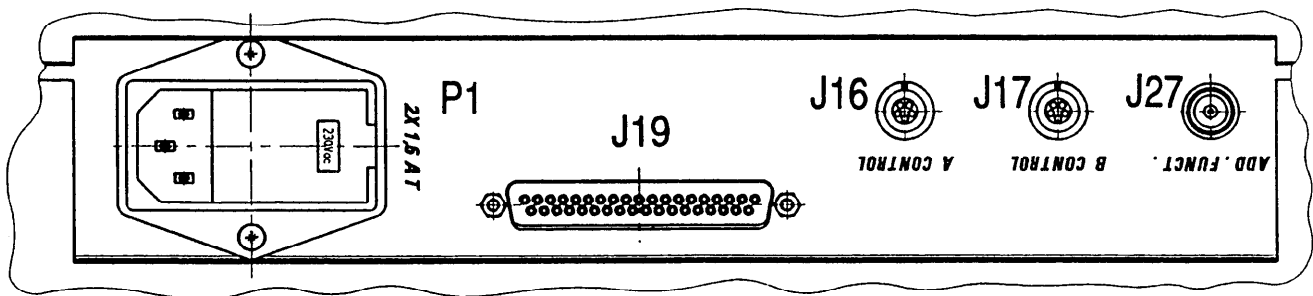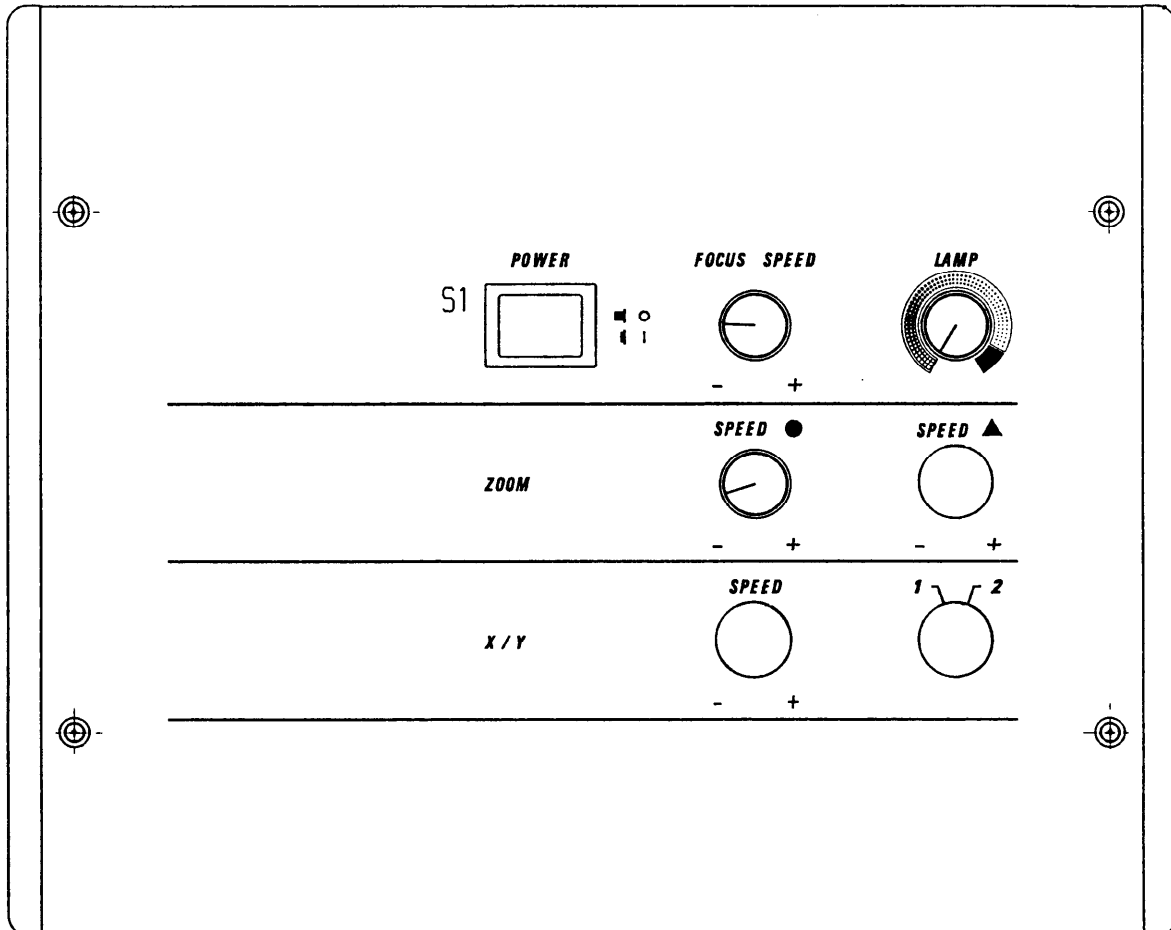


Steuergerät MEL64/65 - Anschlussplatte
Control mit MEL64/65 - Connector panel

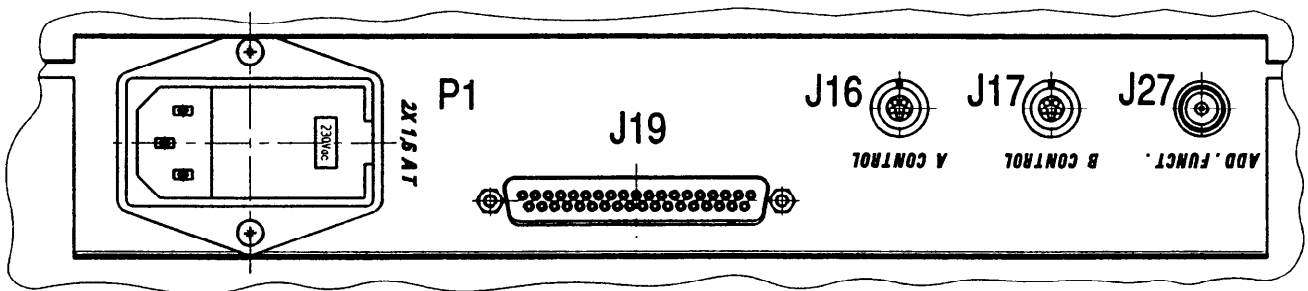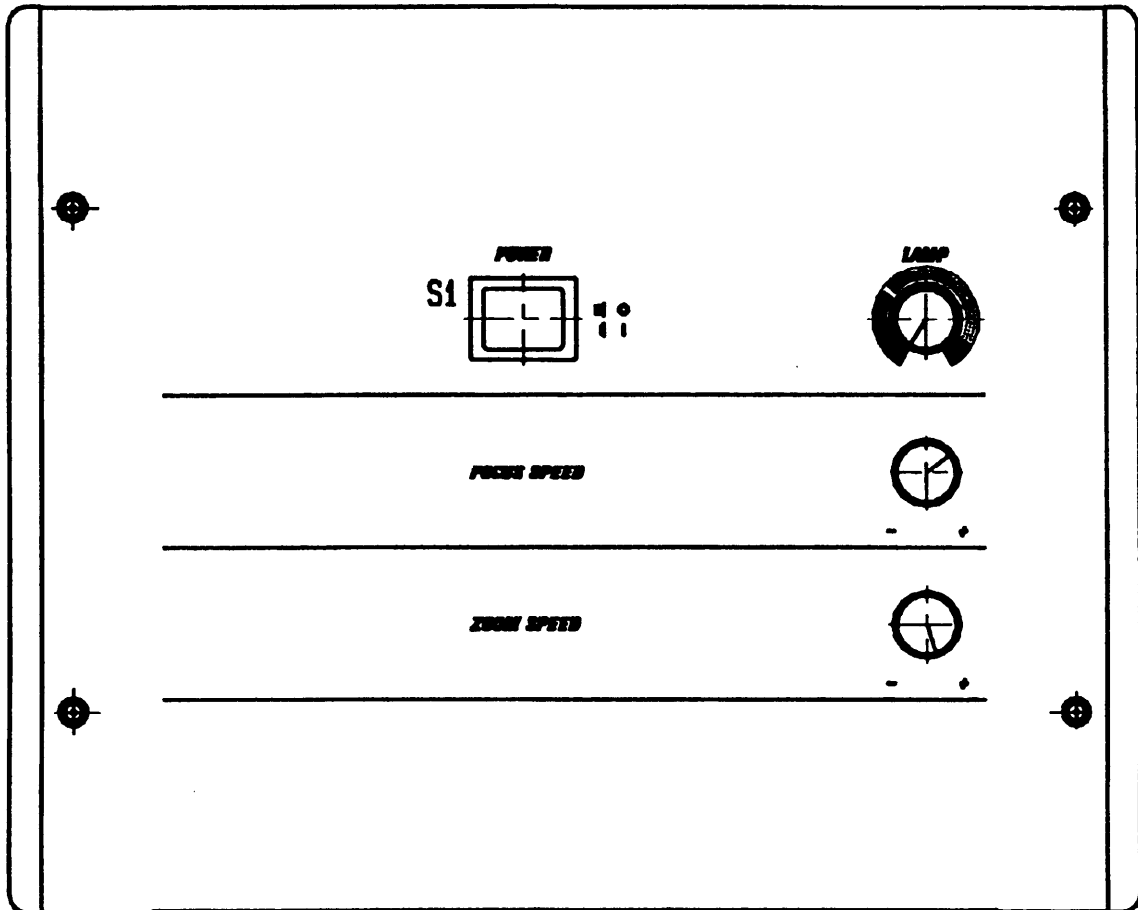


Steuergerät MEL61/62 und MEL64/65 - Rückwand
Control unit MEL61/62 and MEL64/65 - Rear section

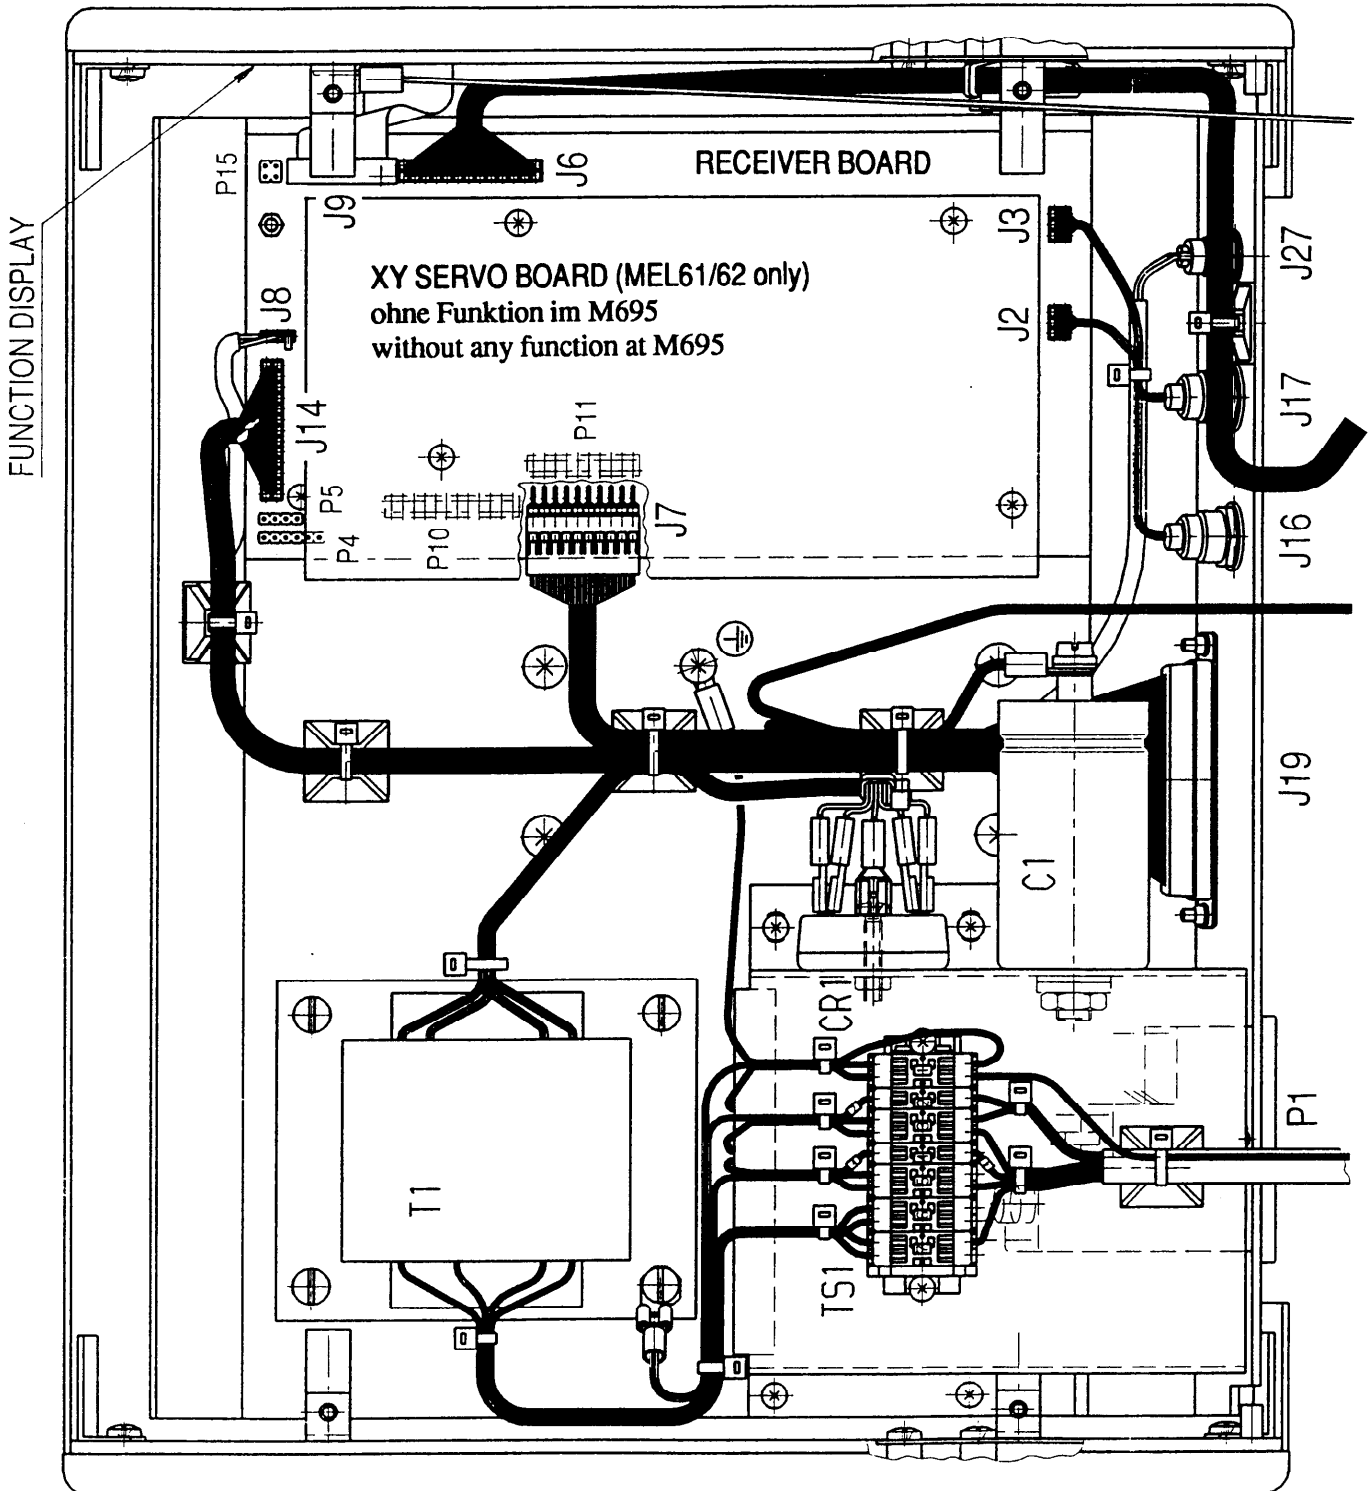


Steuergerät MEL61/62 und MEL64/65 - Front
Control unit MEL61/62 and MEL64/65 - Front section

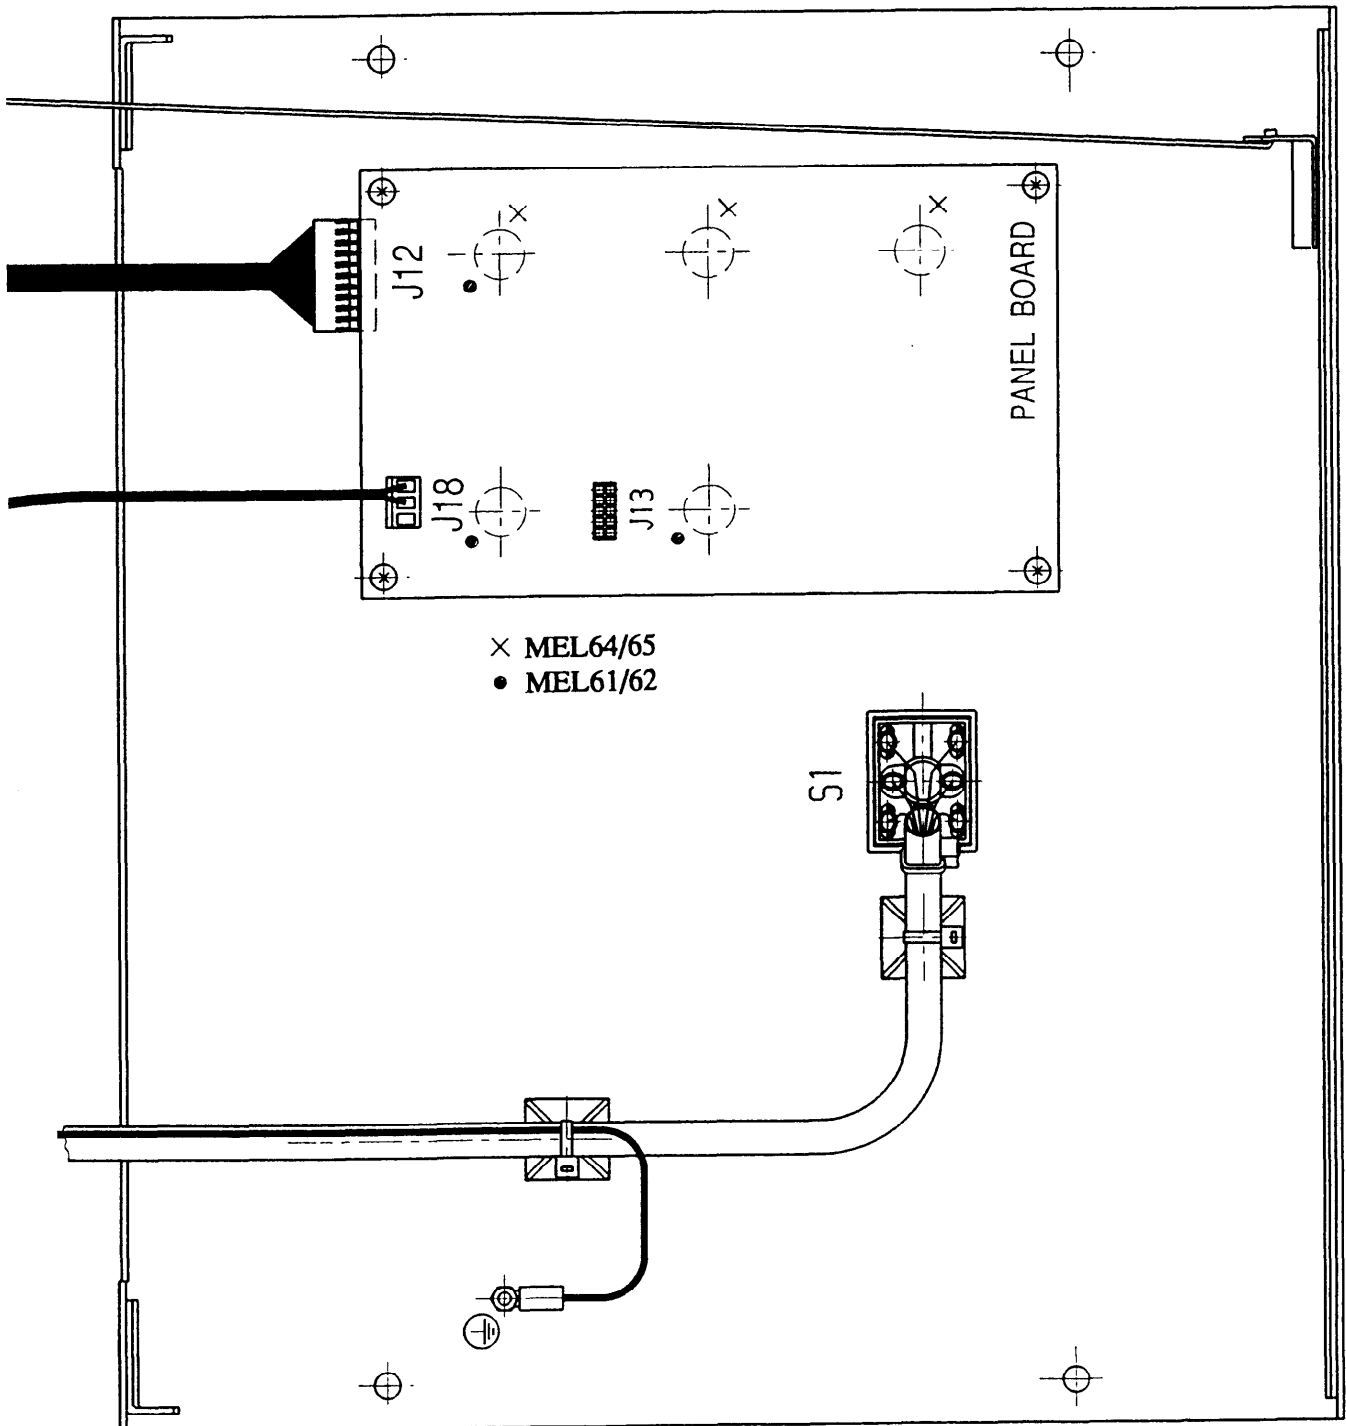


Schwenkarmkabel - Stecker zum Steuergerät
Swing arm cable - Connector to control unit

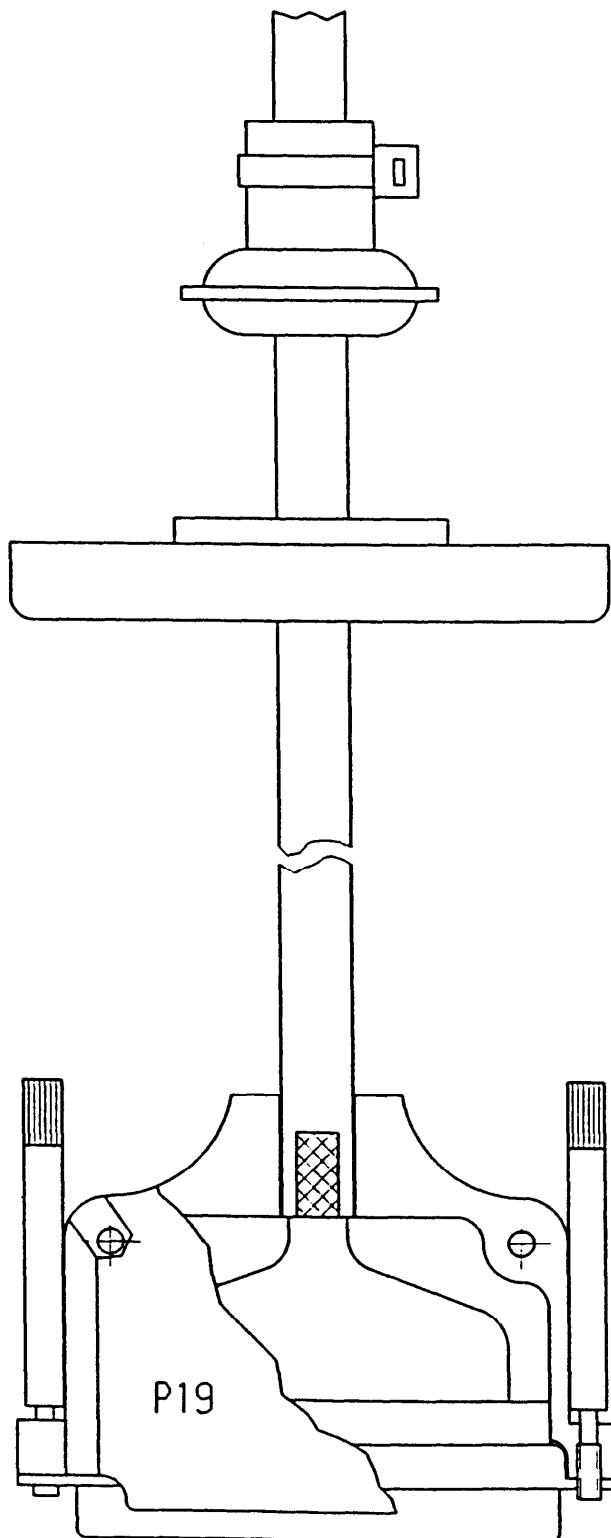


Schwenkarmkabel - Stecker zum Mikroskop M695
Swing arm cable - Connector to microscope M695

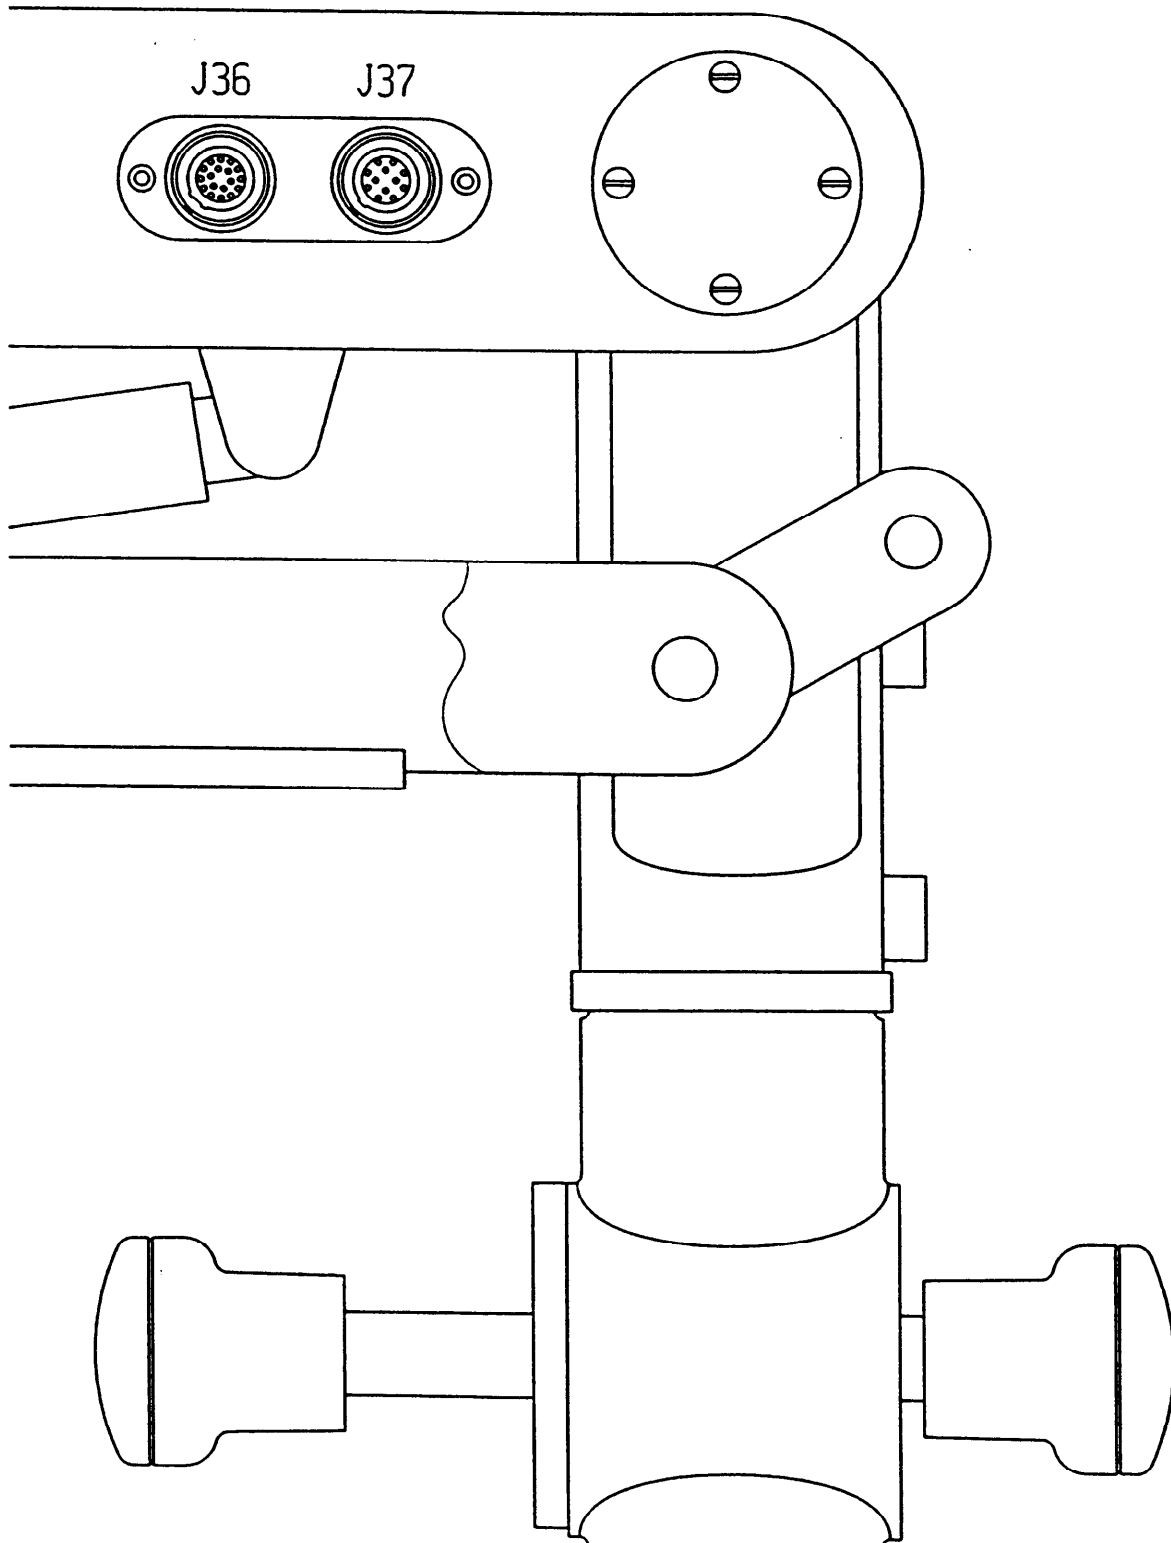


Mikroskop M695 - Ansicht auf U-Träger
Microscope M695 - View to U-carrier

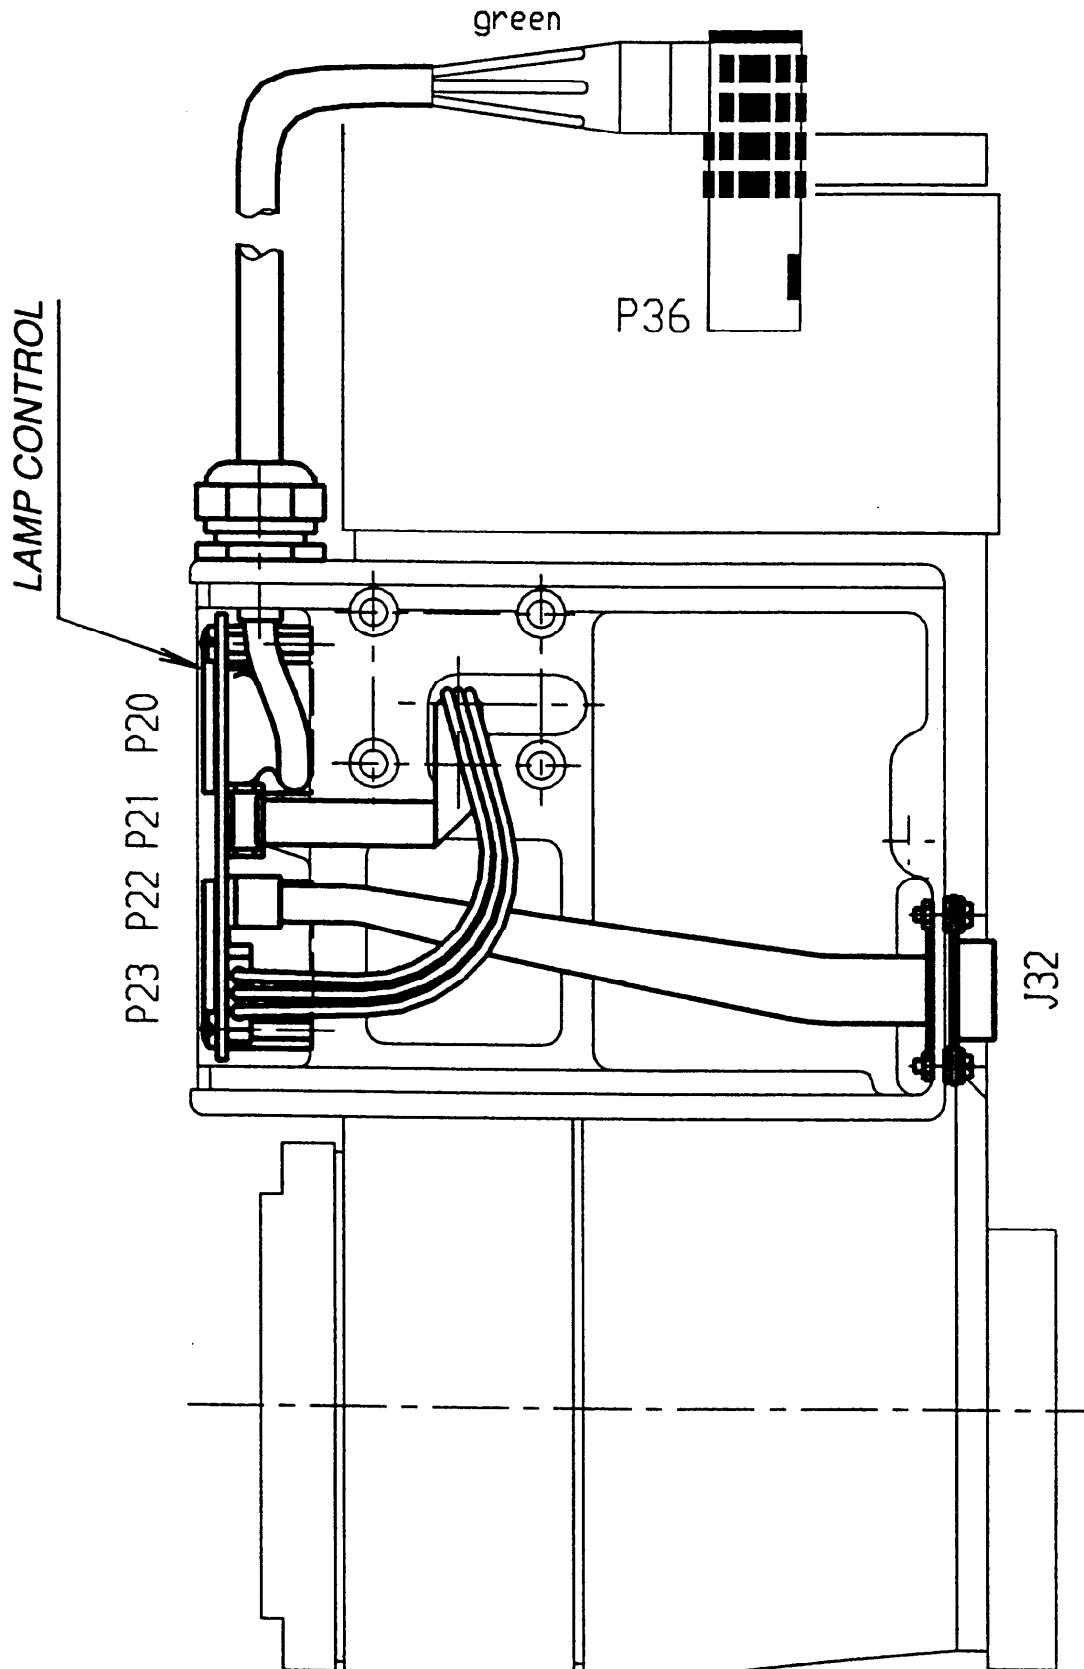

Mikroskop M680 - Ansicht auf Zoom Servo
Microscope M680 - View to zoom servo

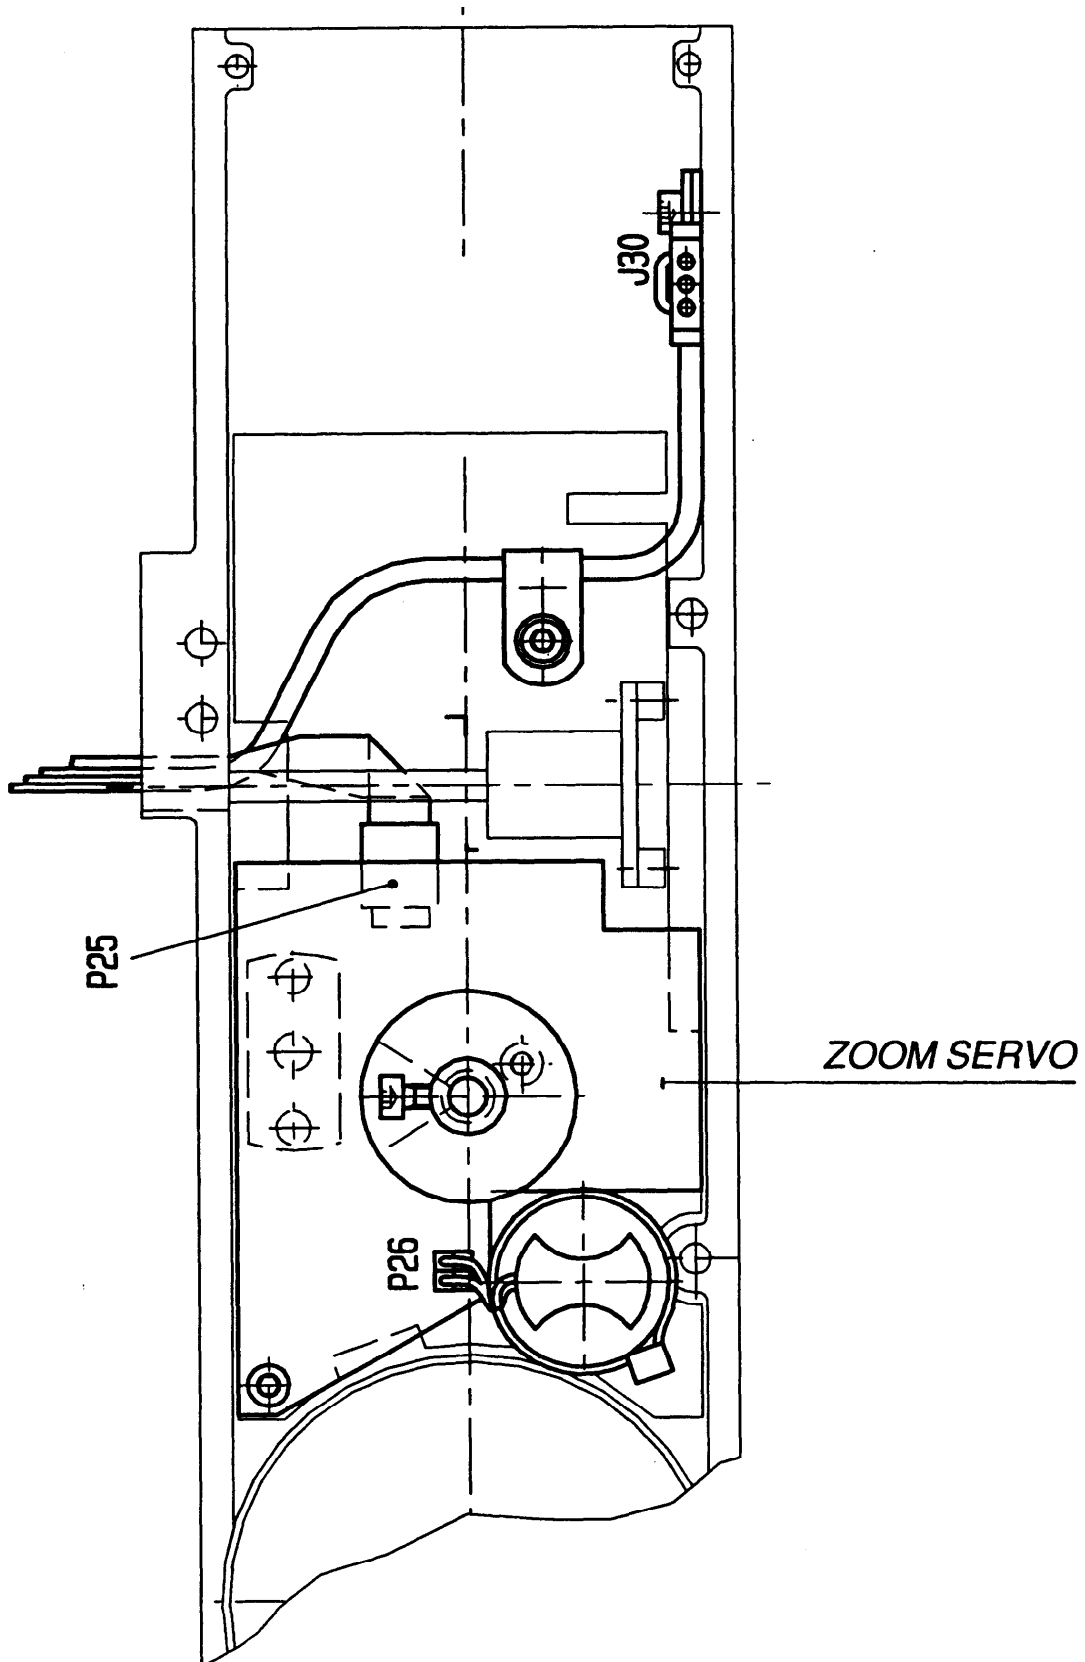

Mikroskop M695 - Ansicht auf motorische Fokussierung (MOB)
Microscope M695 - View motorized focusing (MOB)

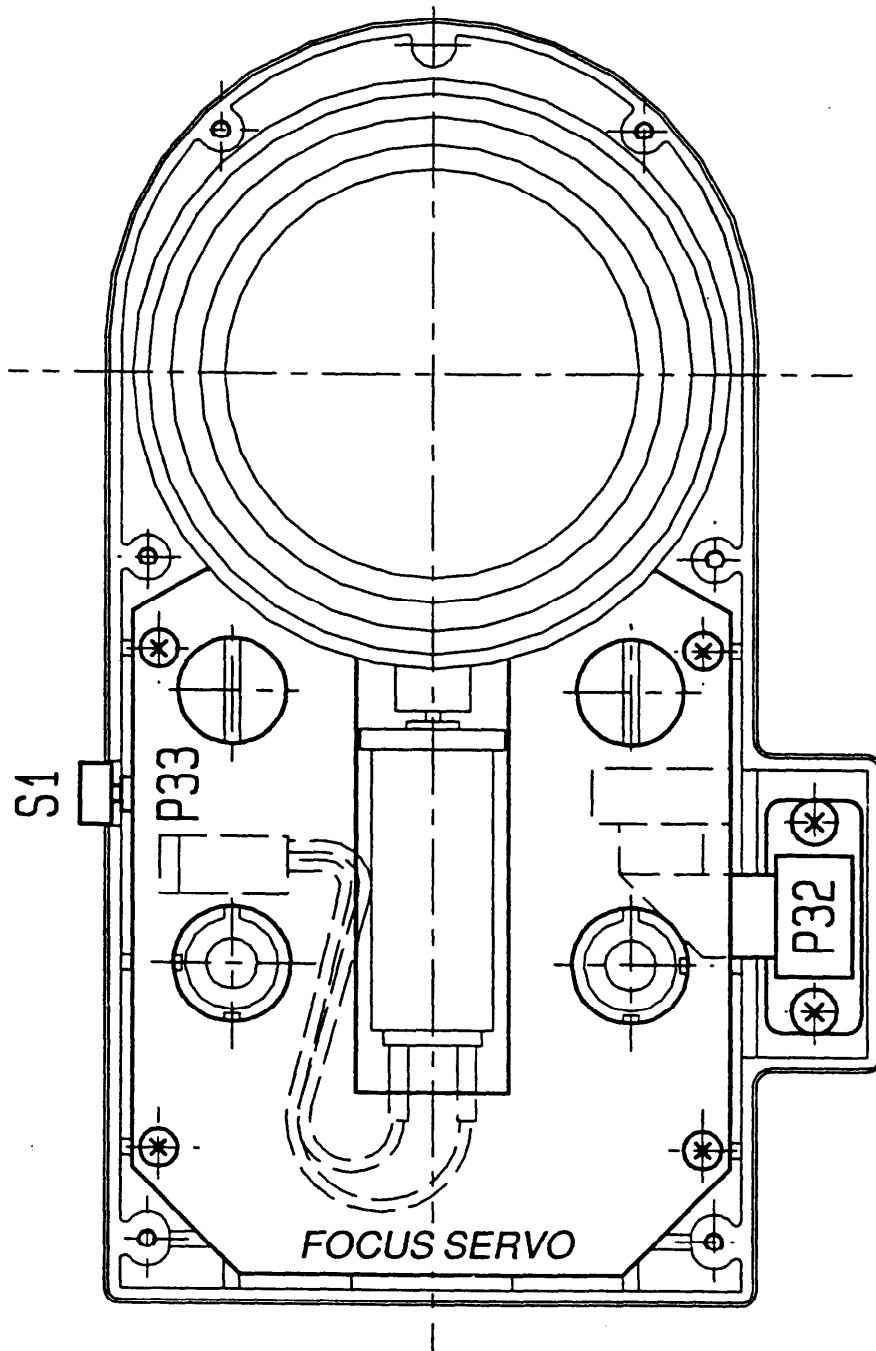

Contents


	<i>Page</i>
Replace X-Y slide	10-1
Replace gas spring of swingarm	10-2
Replacing swingarm cable	10-5


Replace X-Y slide

Remove 2 screws (1) and cover (2).
Remove 6 hollow screws (3) and X-Y slide (4).



After each manipulation, inspect the functioning.

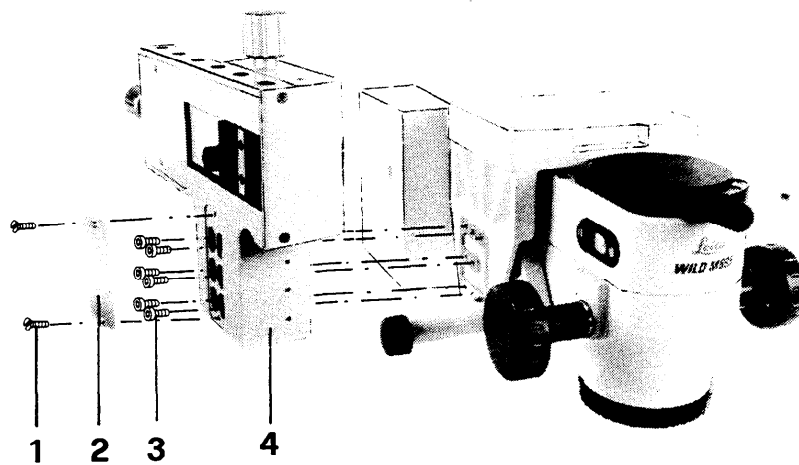



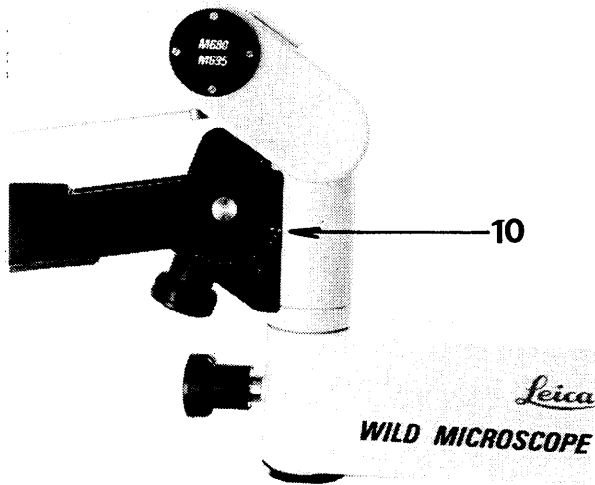


Replace gas spring of swingarm MSV136/137




Set counterbalance to "10". Remove 2 screws (1) and parallel bar (2). Remove washer (3) and parking piece (4).

Note:

The hole-to-hole distance of the parallel bar can be set by turning the eccentric sleeve (5)

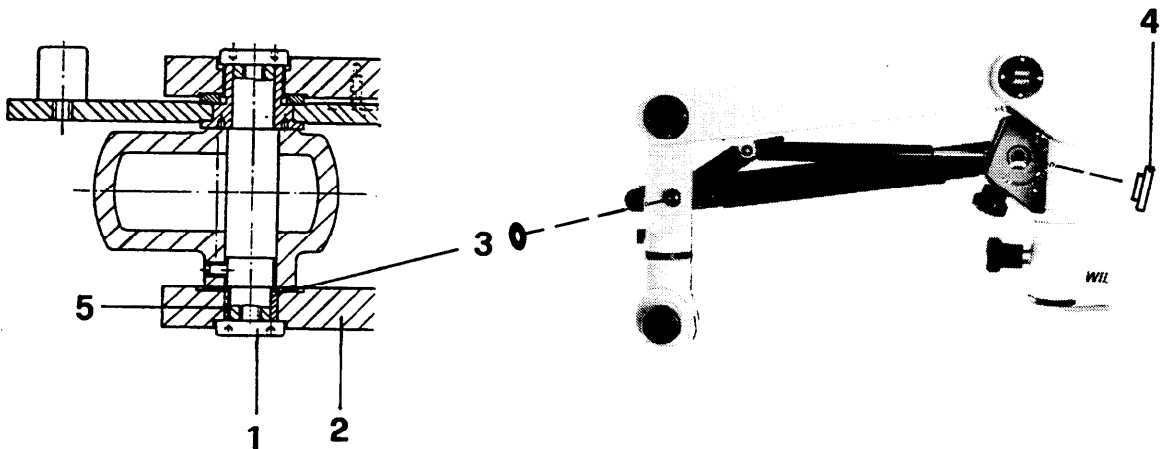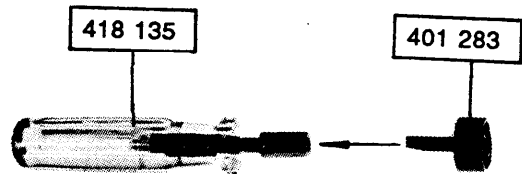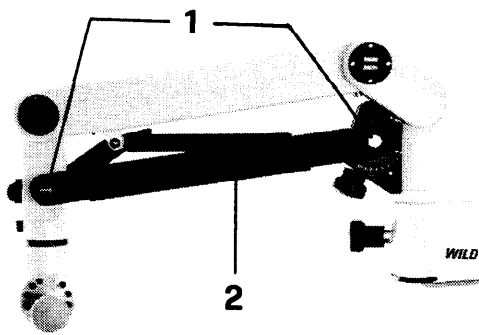


Release screw (1), disengage safety hook (2).
Pull swingarm down until spindle (3) and screw (4) are tension-free.
Remove spindle (3), screw (4) and parallel bar (5).

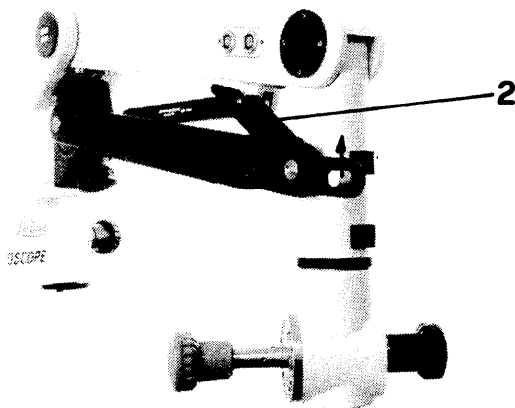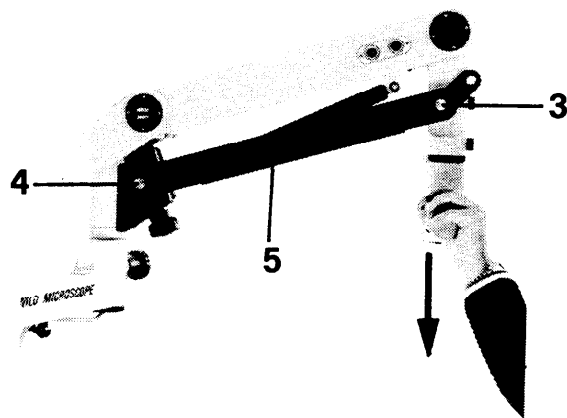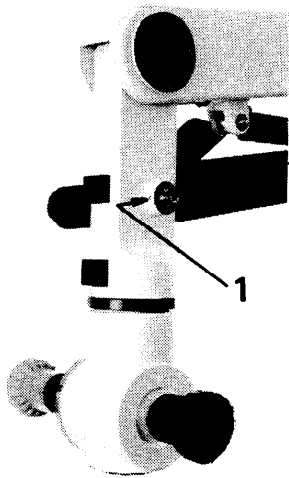

Remove spacer ring (1), safety ring (2) and pin (3).

Assembly:



Fit pin (3) with longer end towards safety hook.

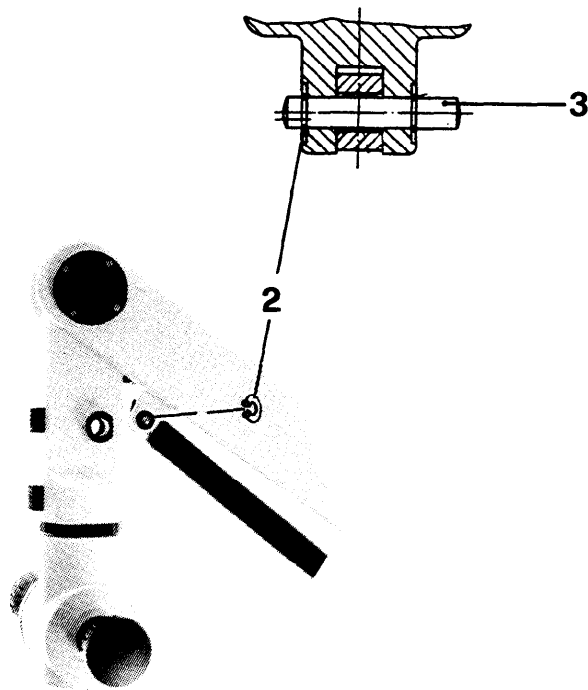


Remove gas spring (4) from mount (5) and unscrew it.

Assembly:

Screw gas spring fully in and then unscrew by up to 1/2 turn until swingarm bearing and gas-spring bearing coincide.

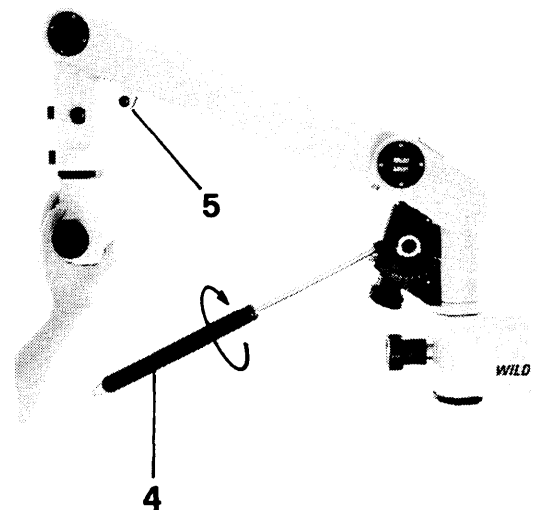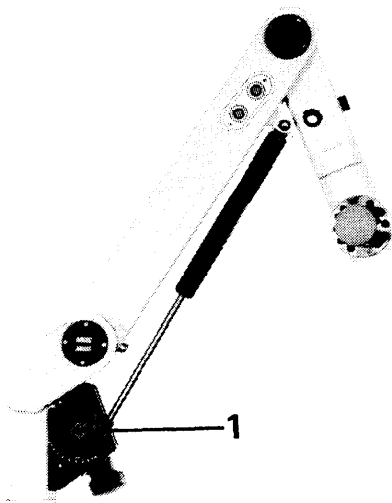

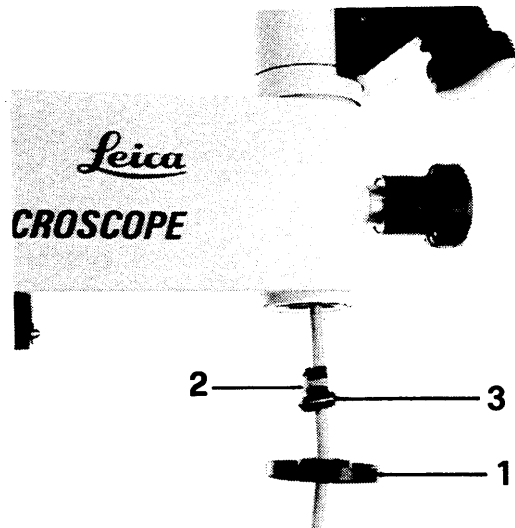

Replacing swingarm cable

Screw off cover ring (1) and cut off cable tie (2) from cable duct (3).

Remove 2 screws (4) and extract plug plate (5) complete with Lemo plug.

Open AMP plug and push contact pins out to the rear.

Pull cable out from swingarm.




Note:

Tie a 1.5-metre long string to the cable so that it is easier to pull in.

Assembly:



Bundle together the contact pins of the new cable and bind them with adhesive tape. Raise the swingarm to its highest position and pull in the cable.

Secure cable duct (3) with a cable tie, one metre away from the AMP plug.

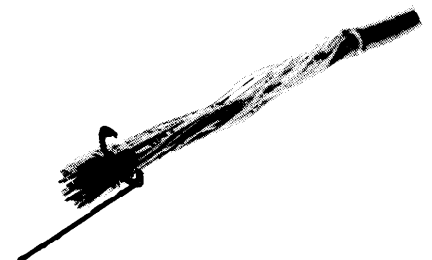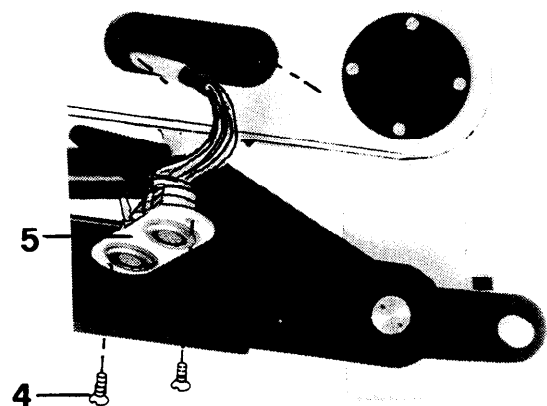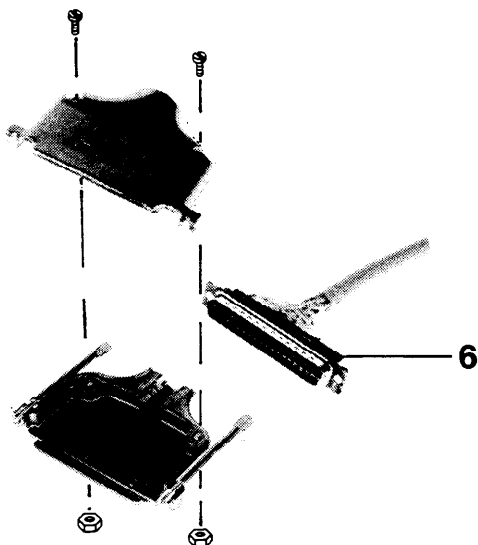


Inspect continuity of contacts in J36 and J37.


Plug wires into socket strip P19 in accordance with diagram.

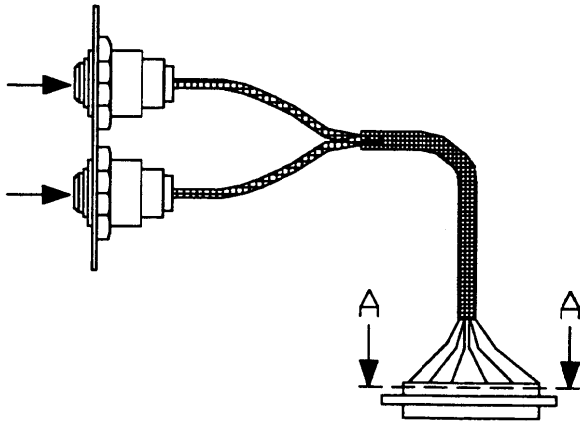

J36



J37

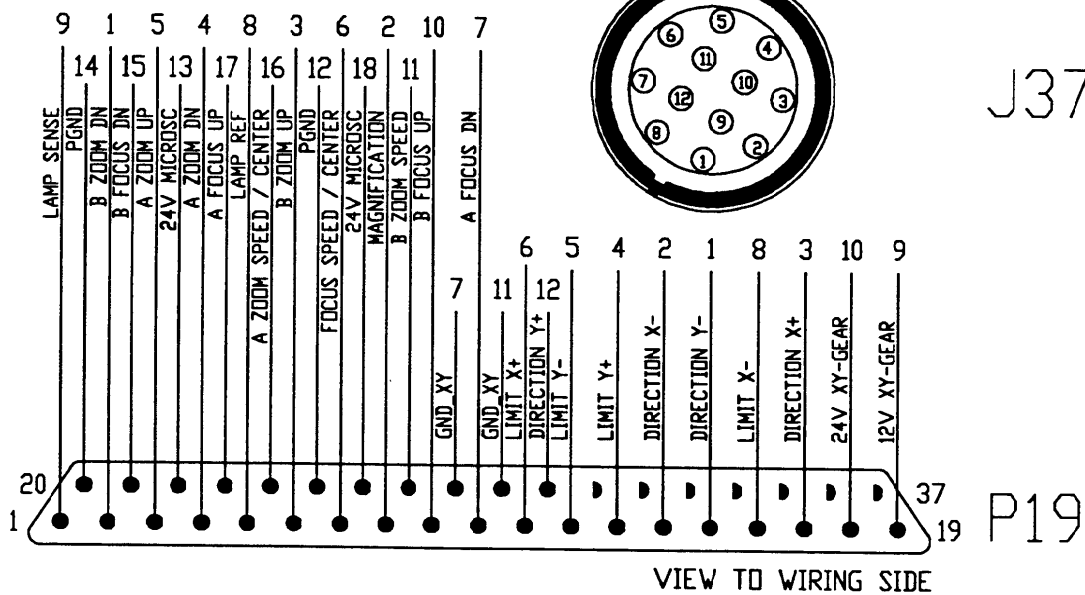

P19

VIEW TO WIRING SIDE

A - A

Contents


	<i>Page</i>
Motorized focusing	
Focus servo board	11-1
M695	
Replace lamp-control board	11-2
Control unit	
Replacing panel board	11-3
Replacing receiver board	11-4
Replacing display board	11-4

Motorized focusing



Focus servo board for motorized focusing

Remove 6 screws (1), adapter (2) and upper part of housing (3).

Remove 6 screws (4). Raise focus servo board (5). Pull out plug J33.

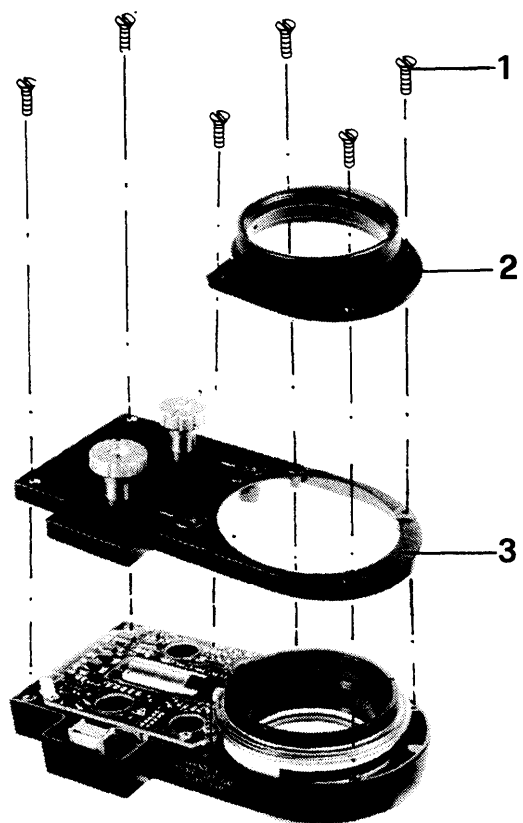

After each manipulation, inspect the functioning.



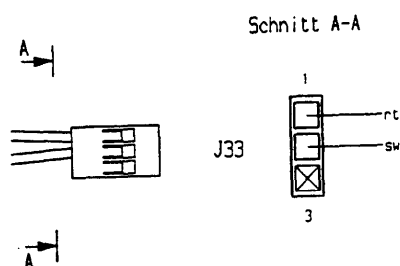
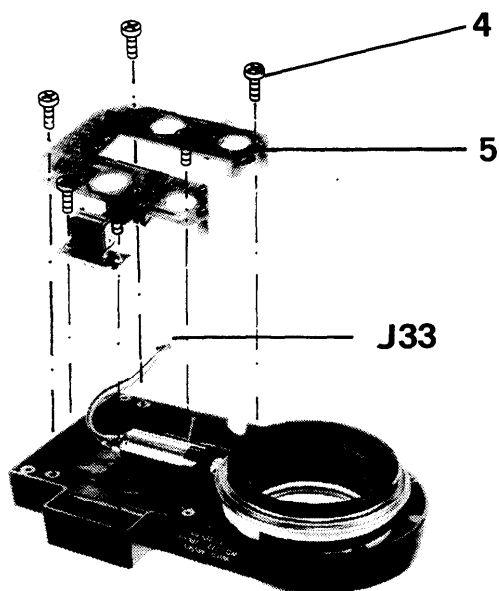


M695 optics carrier


Replace lamp-control board

Remove 3 screws (1) and bracket (2).

Pull out 4 plugs (3), Remove 2 countersunk screws (4), 2 cheese-head screws (5) and the lamp-control board (6).

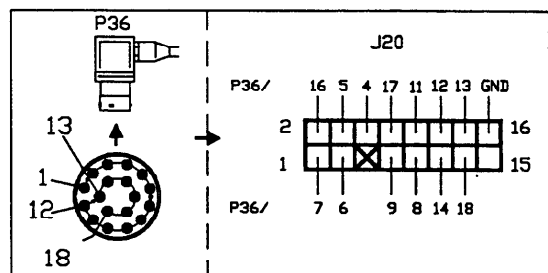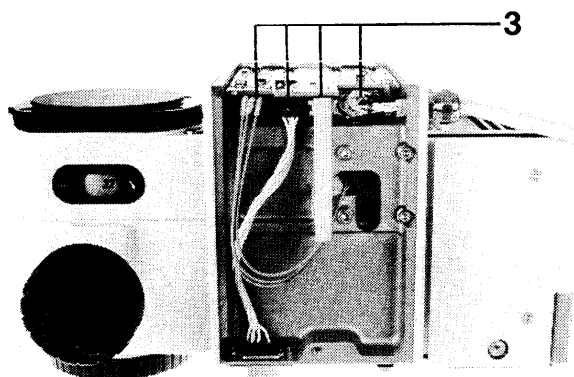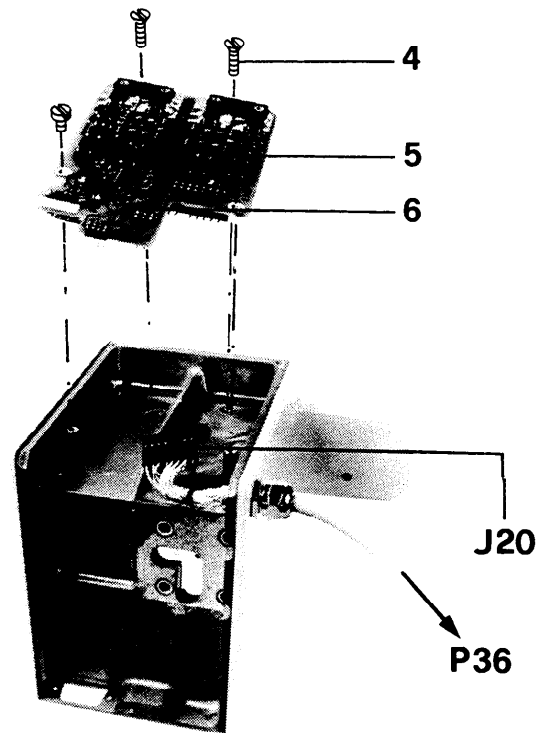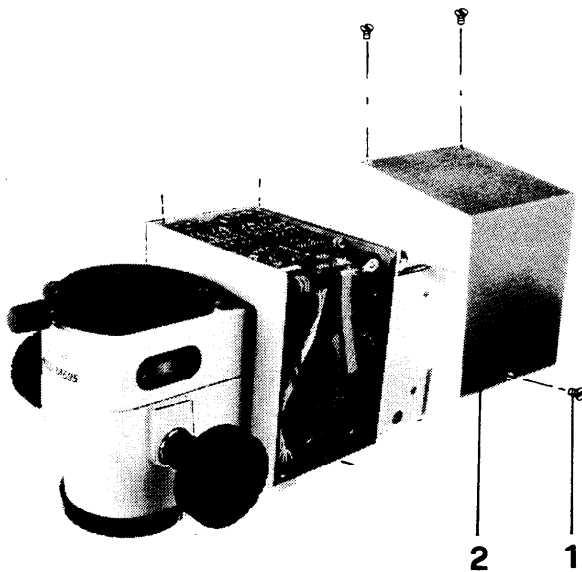

Control unit MEL64/65

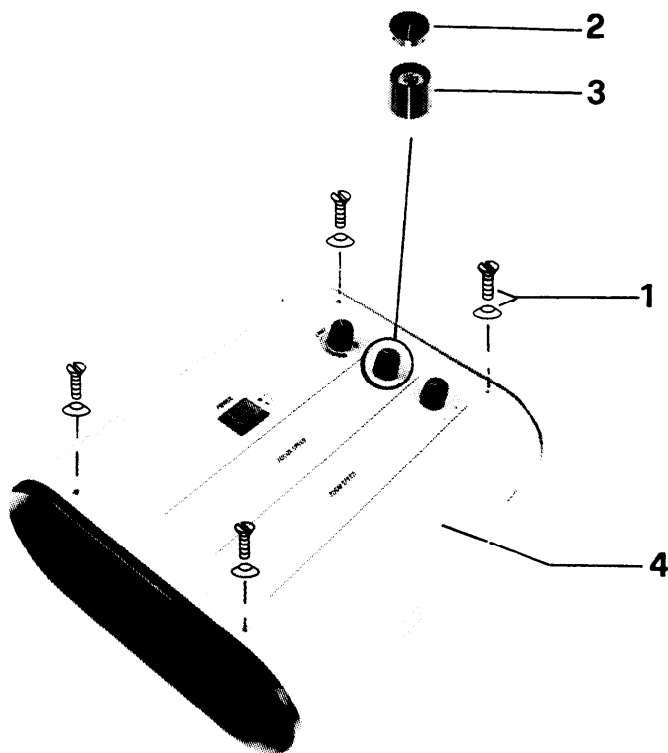

Replacing panel board



Remove 4 screws with washers (1). Remove knob cover (2) and knobs (3). Open front cover (4).

Pull out 2 plugs. Unscrew and remove 4 screws (5). Remove panel board (6).

Assembly:


The maximum permissible gap between knobs and front cover is 0.5mm.

Adjust the rotation range of the knobs.

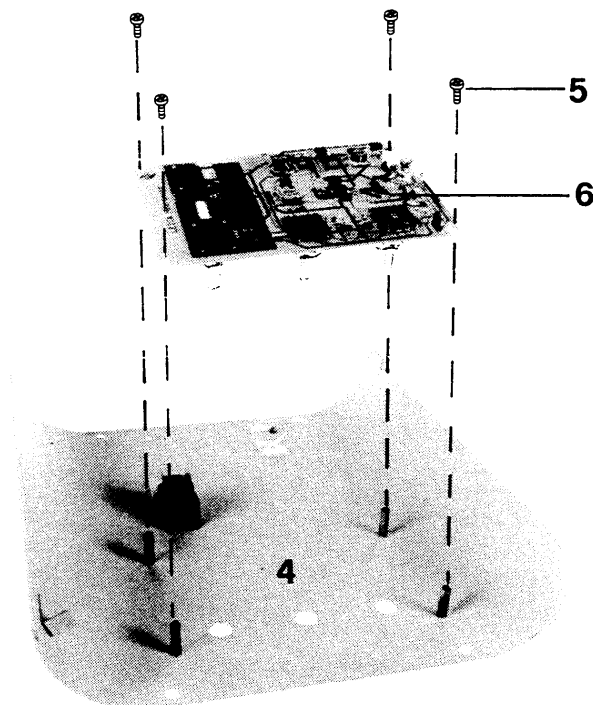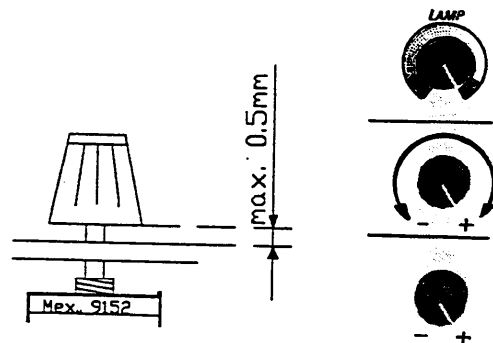

Replacing receiver board


Remove spacer nut (1). Pull plug out from receiver board (2). Remove receiver board.

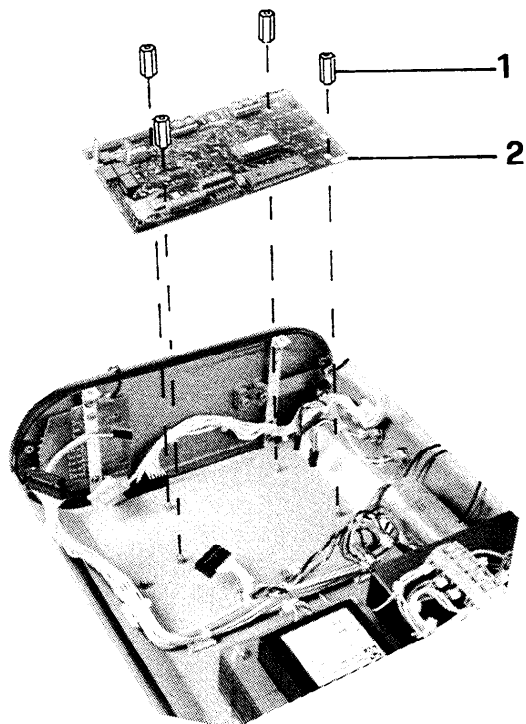

Replacing display board

Remove 2 screws with washers (3), and take out function display (4)

Assembly:
Align LEDs with display window.

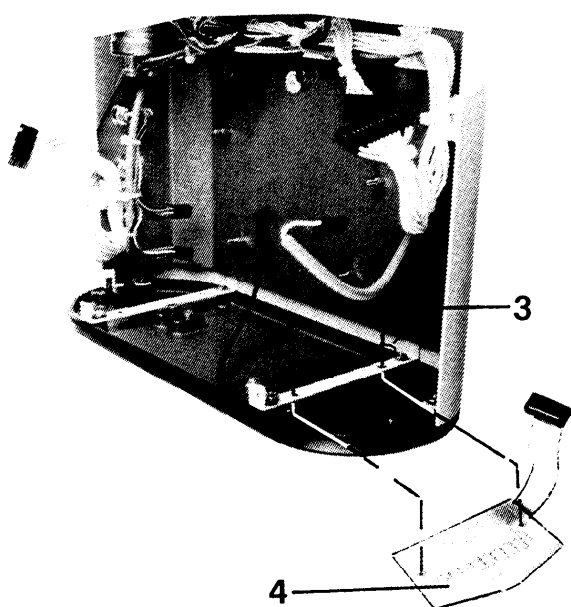

Contents

Section	Page
1. Inspecting the hand- / footswitch functions and function display on the MEL64/65:	12-1
2. Lamp control:	12-4
3. ZOOM control:	12-4
4. FOCUS control:	12-5
5. Optics	12-6
6. Tilttable joint / swingarm	12-6
Test report	12-7

Test plan for M695 surgical microscope



Always pull out the power plug before opening the control unit!

Assemble the M695 surgical microscope in accordance with the user manual, but disconnect all cables.

Inspect the M695 system, using the test box (Test set M695/M680, stock no. 566 152)

1. Inspecting the hand- / footswitch functions and function display on the MEL64/65:

1.1 Connect the hand- / footswitch (6 functions) and the power plug to the MEL 64/65.

- The plugs must go in and out without difficulty.

1.2 Activate the power switch of the MEL64/65.

- The control unit switches on and the indicator lamp in the power switch shines.
- The 5V LED on the function display shines.
- The ML LED on the function display shines.

If the control unit does not switch on:

Inspect the power cable and the power connection

Inspect the fuse on the panel board inside the control unit

(see wiring plan in section 9 and power unit defect search procedure on page 4-3)




(Power unit defect search procedure, page 4-3)

1.3 Activate the foot- or handswitch functions.

- The appropriate LED on the function display shines.
(If a fault arises, exchange the foot- or handswitch and repeat the inspection procedure.
If there is still a fault, then its source is to be found in the MEL64/65 control unit.)

(Fault location in hand-/footswitch functions, page 4-4)

ML on/off
Microscope lamp M L
A on/off
Additional illumination A
Focus up
Focus down F ↓
Zoom up Z ↑
Zoom down Z ↓

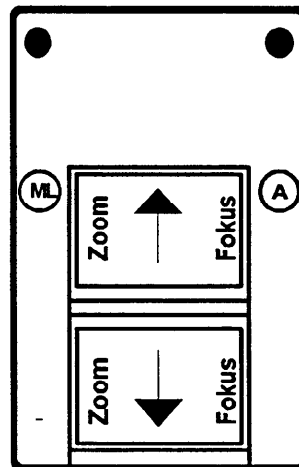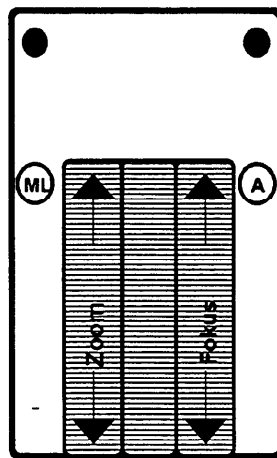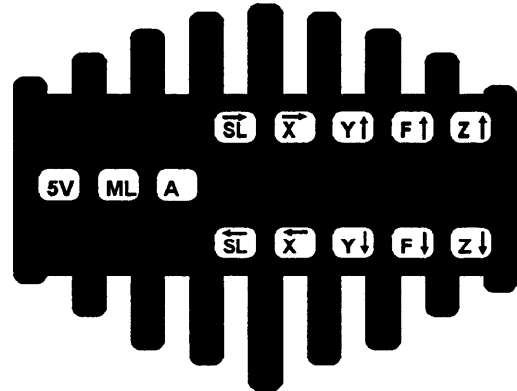


1.4 Connect cables of microscope and swingarm,

- The plugs must go in and out without difficulty.

Preparation: Connect test box.

- Separate plug connection J/P36 on swingarm.
- Hang test box on to swingarm. Connect plug P36 from test box to swingarm, and from M695 microscope to test box.
- Set test box switch "MICROSCOPE SELECT" to **A**.

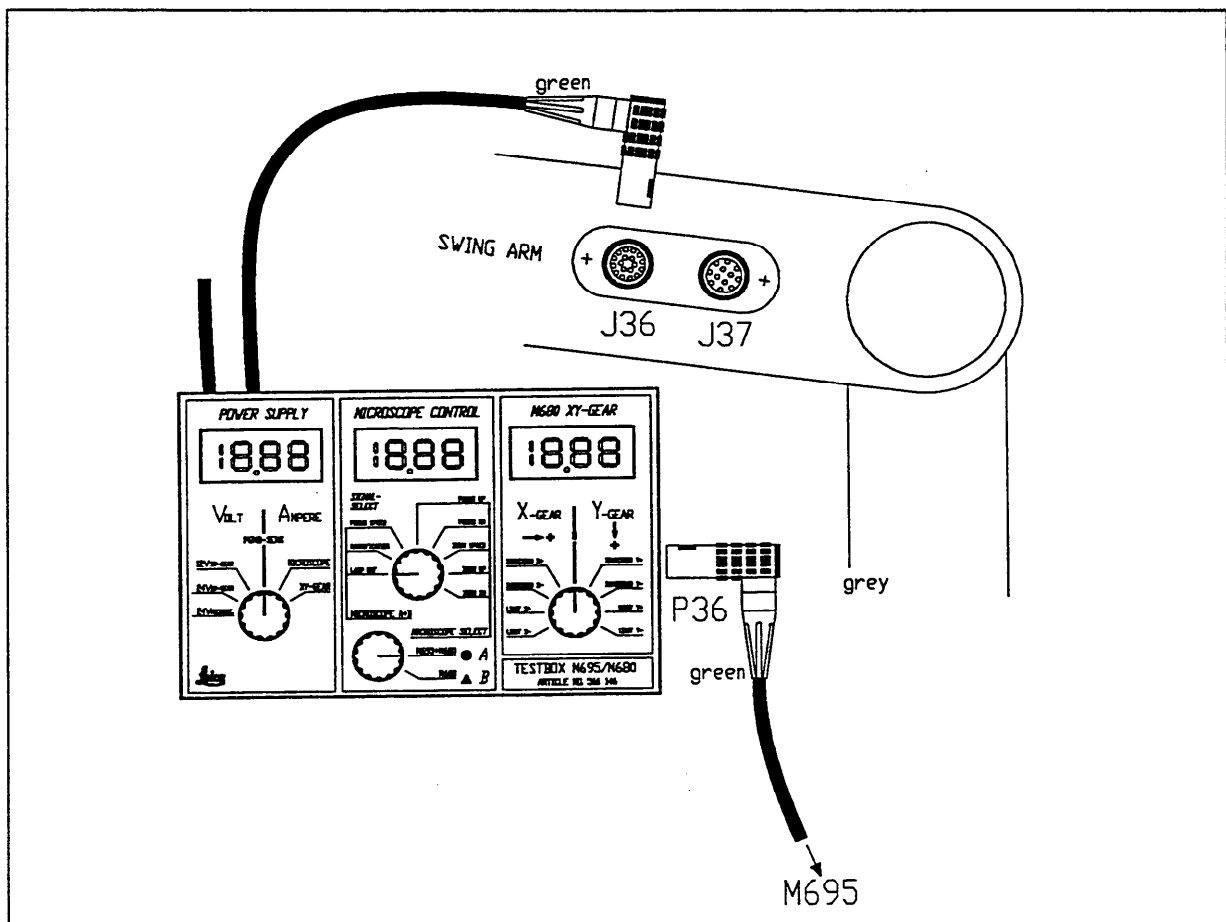

2. Lamp control:

2.1 Turn LAMP potentiometer on control unit from min. to max.

- Reading on test box: LAMP REF. min./max. 0.3.....5v.

The brightness of the microscope lamp is continuously adjustable.

2.2 Activate the quick-change lamp mount.

- The spare bulb is moved into the beam path, and lights up.
- The orange indicator springs out.
(Push the orange indicator back into the rear wall)

(Fault location in lamp control: page 4-7)

Important: Before proceeding further with the test, reset the lamp to its minimum brightness.

3. ZOOM control:

3.1 Turn the ZOOM SPEED potentiometer from min. to max. and from max. to min.

- Reading on test box: ZOOM SPEED min./max 1.84...2.34V15V ±5%

The zoom speed is continuously adjustable.

3.2 Use foot-/handswitch to activate ZOOM UP.

- Reading on test box: ZOOM UP Low/High <0.2V/>4.75V

3.3 Use foot-/handswitch to activate ZOOM DN.

- Reading on test box: ZOOM DN Low/High <0.2V/>4.75V


(Fault location in ZOOM control: page 4-8)

3.4 Mechanical zoom movement.

- Zoom moves uniformly in both directions.

3.5 Inspect zoom range.

- Travel to zoom end positions 7 and 36 using max. SPEED. Zoom should not touch mechanical stop. Relevant magnification is seen centred in window.

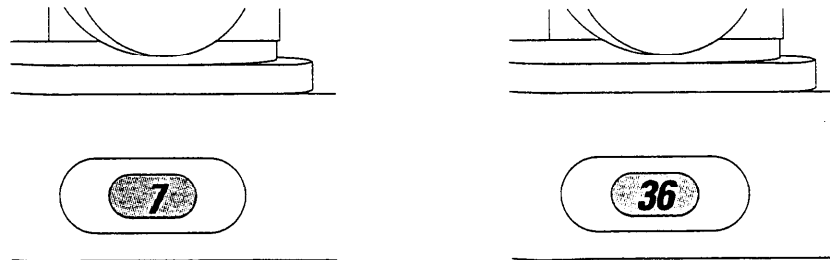

4. FOCUS control:

4.1 Turn FOCUS SPEED potentiometer from min. to max. and from max. to min.

- Reading on test box: FOCUS SPEED min./max. 1.25...1.7V/5V $\pm 5\%$
The focus speed is continuously adjustable.

4.2 Use foot-/handswitch to FOCUS UP.

- Reading on test box: FOCUS UP Low/High <0.2V/>4.75V

4.3 Use foot-/handswitch to FOCUS DN.

- Reading on test box: FOCUS DN Low/High <0.2V/>4.75V

(Fault location in FOCUS control: page 4-9)

4.4 Mechanical focus movement

- Focus moves uniformly in both directions.

4.5 Activate yellow knob on motorized focusing: FOCUS reset

- Focus automatically returns to basic position.
(Use FOCUS UP and DN to travel away from basic position, and repeat test)

5. Optics

5.1 Cleanliness of optical components

- All surfaces of optical components in the observation and illumination beam paths must be clean,

5.2 Zoom

- Focus on the object and operate ZOOM UP and ZOOM DOWN at their minimum speeds.
The image sharpness should remain constant over the entire zoom range.
- 1 The image should not jump suddenly when ZOOM UP and ZOOM DOWN are being operated.

6. Tilttable joint / swingarm

6.1 Rotation

- The tilttable joint must be easily and smoothly tumbable after the brake has been released.

6.2 Brakes

- As the braking knob is applied, the movement becomes steadily less free and finally the joint locks completely. When the brake knob is turned the other way, the movement steadily becomes easier.

6.3 Clip-on handles

- The sterilizable clip-on handles must be convenient to put on and take off again. They must click in and out perfectly.

6.4 Gas spring

- The vertical adjustment must be smoothly adjustable from one end to the other.
- At maximum loading, and with the weight compensation at 10, the swingarm must not drift downwards.

6.5 Weight compensation

- The adjusting spindle must be adjustable from 0 to 10.

6.6 Safety hook

- The safety hook must engage faultlessly. When it is moved sideways, the ratchet bolt must remain in position.

Test report for M695 surgical microscope

Customer: _____

Tested by: _____

Date: _____

<i>Stock no.</i>	<i>Description</i>	<i>Serial no.</i>
445 560	Optics carrier M695
445 561	Microscope carrier 45°
445 562	Microscope carrier 45°/70°
445 494	Swingarm MSV136 for floor stand
445 740	Swingarm MSV167 for ceiling mount
445 551	Control unit MEL64 for floor stand
445 552	Control unit MEL65 for ceiling mount
445 365	Objective, mot. foe., f=250mm
445 563	Objective, mot. foe., f=325mm
445 564	Objective, mot. foe., f=275mm
.....	Footswitch (6 functions)
445 203	Handswitch (12 functionsn)
.....	Binocular tube MTU

Other accessories:

.....
.....
.....
.....

Test report for M695

Tested

1.	Test hand-or footswitch functions and function display on MEL64/65:			
1.1	Connections, hand-/footswitch, power plug			
1.2	Power switch MEL64/65			
	LED 5V			
	LED ML			
1.3	Foot-/handswitch functions			
	ML on/off /			
	A on/off /			
	F↑ / Focus up			
	F↓ / Focus down			
	Z↑ / Zoom up			
	Z↓ / Zoom down			
1.4	Connections, microscope and swingarm cable			
2.	Lamp control			
2.1	LAMP potentiometer function min./max.			
	LAMP REF.		min. V	max. V
2.2	Quick-change lamp mount			
	Spare bulb			
	Orange indicator			
3.	ZOOM control			
3.1	ZOOM potentiometer function min./max.			
	ZOOM SPEED		min. V	max. V
3.2	ZOOM UP		Low V	High V
3.3	ZOOM DN		Low V	High V
3.4	Mechanical running of zoom			
3.5	Zoom range (7x to 36x)			
4.	FOCUS control			
4.1	FOCUS potentiometer function min./max.			
	FOCUS SPEED		min. V	max. V
4.2	FOCUS UP		Low V	High V
4.3	FOCUS DN		Low V	High V
4.4	Mechanical running of focus			
4.5	Basic focus position			
5.	Optical components			
5.1	Cleanliness of optical components			
5.2	Image sharpness / zoom range			
6.	Tiltable joint/swingarm			
6.1	Revolution of joint			
6.2	Brakes			
6.3	Clip-on handles			
6.4	Gas spring			
6.5	Weight compensation			
6.6	Safety hook			

M695 service courses

Content:	Assembling the microscope on the floor stand Exchanging modules and boards Replacing the gas spring in the swingar Using the test box to locate faults
Goals:	After the course, the participant should be able to <ul style="list-style-type: none">- install the instrument ready for use- use the test box to locate faults- exchange modules and boards in accordance with the instructions- carry out a comprehensive inspection of the functions
Location:	Leica AG, Heerbrugg, Service LSG/MSM training department In agencies, provided that the service technician (instructor) has already attended an M695 course at Leica AG in Heerbrugg
Duration:	2 days
Cost:	In accordance with present guidelines, described in the Service Training Program (excluding travel and accomodation).
Technical Requirements:	Basic knowledge of mechanical engineering and of measuring technique
Number of participants:	Individuell
Remarks:	Send application to agency

Test set M695/M680 - stock no. 566 152

Contents of test set

- Test box, stockno. 566 146
- Service cable M695/M680, stock no. 566 148
- Service handswitch, stock no. 566 147

Enables defective assemblies to be identified

- Foot- or handswitch
- Swingarm
- Control unit MEL61/62 and MEL64/65
- X- or Y-gear MSV138 (M680 only)
- M695/M680 microscope

Procedure for fault location ***See section 4***

1. Introduce the test box between the swingarm and the microscope - Plug connections JP36 and JP37.
2. Inspect the voltages and currents of the POWER SUPPLY as described in Section 4.

Cause in footswitch?

3. Substitute service handswitch for footswitch, observe signal voltages, and also monitor LEDs on control unit.
4. Observe the signal voltages of the defective function (MICROSCOPE CONTROL or XY-gear) - as described in Section 4.

Cause in microscope of in XY-gear?

5. Separate the microscope or the XY-gear, as appropriate, from the test box, and observe the signal voltages which flow from the control unit through the swingarm.

Cause in control unit or swingarm?

6. Use service cable to bridge swingarm, and observe signal voltages from control unit.

Functions of test box

All control voltages . . .

All supply- and control voltages between the control unit and the microscope with XY-gear can be measured.


. . . to the microscope . . .

Control voltages to the microscope are measured relative to XY_GND, such to the XY-gear relative to GND_XY.

. . . measure at low light level

Unless otherwise indicated, set the lamp to minimum brightness. The voltages indicated in Section 4 are only valid for this condition.

Voltage levels are falsified by the voltage drop between the control unit and the microscope. Because of the current taken by the lamp, this voltage drop to PGND (measuring ground) can be as much as 0.9V. The control voltages of focus and zoom are measured against PGND and are therefore influenced.

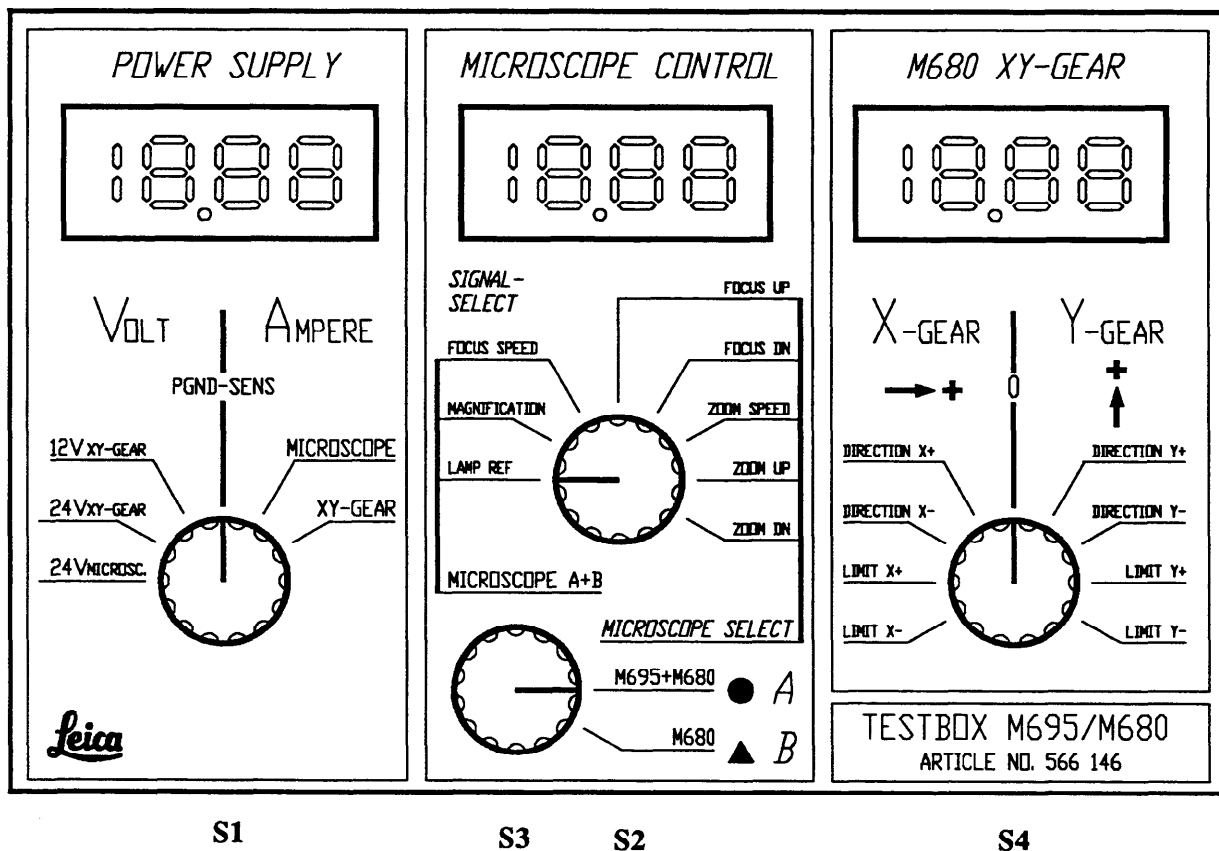

**The test box:
three multimeters**

One digital voltmeter is assigned to each of the functions **POWER SUPPLY**, **MICROSCOPE CONTROL** and **XY-GEAR**. The signals reach the measuring instrument through a rotary switch.

Digital voltmeters

Range of measurement: 1.999V - with overflow display (OL)
Measurement precision: 1% +- 1 digit, 2 measurements/second
Auxiliary voltage: 7 . . . 15VDC

**Supply for digital
voltmeter
Circuit diagram on
page 18-5**

The power is derived from the 24V supply of the XY-gear (at control unit MEL61/62 only). Three galvanically-separating DC converters each reduce the voltage to approx. 12V each.

Rotary switch S1: Displaces the decimal point on the display by one digit to the right for the 24V - measuring ranges.

**POWER SUPPLY
Diagram on page 18-6**

Rotary switch S1: Level 1 ... Selects current- and voltage ranges.
Voltage distributor: 1/10 for 12V range
1/100 for 24V ranges
Current measurement range: Voltage drop across 0.1 ohm resistor.
Measuring ground: PGND - 24V_{MICROSCOPE}
SENS - PGND
GND-XY - 12V / 24V_{XY-GEAR}

**MICROSCOPE
CONTROL
Diagram on page 18-7**


Rotary switch S3: Selects those signals which are assignable either to microscope A or to microscope B.
Rotary switch S2: Selects the control signals to and from the microscope.
Voltage distributor: 1/10
Measuring ground: SENS


XY-GEAR
(at M680 only)
Diagram on page 18-8

Rotary switch S4:	Selects the signals from and to XY-GEAR.
Voltage distributor:	1/10
Measuring ground:	GND_XY


Specifications:

Voltage measurement:	+3% +-1 digit
Current measurement:	+5% +-1 digit

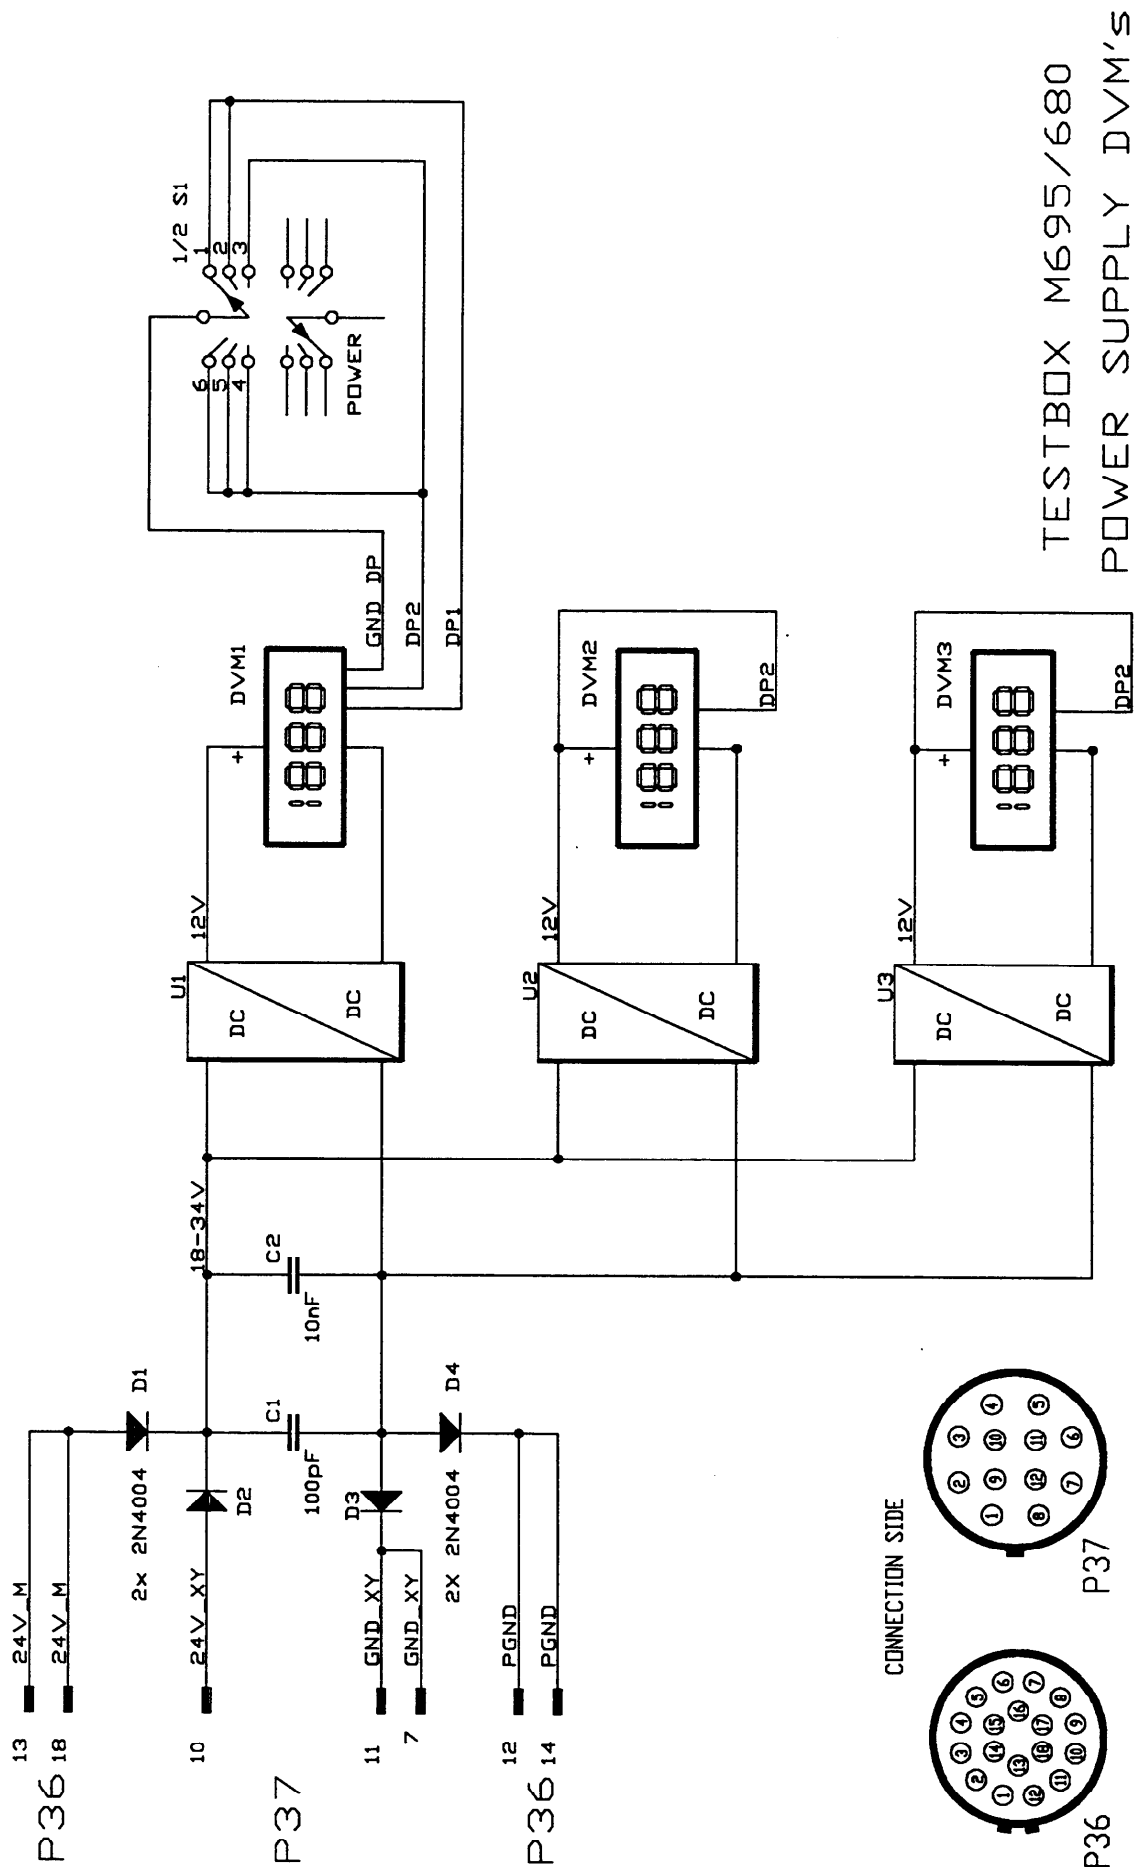

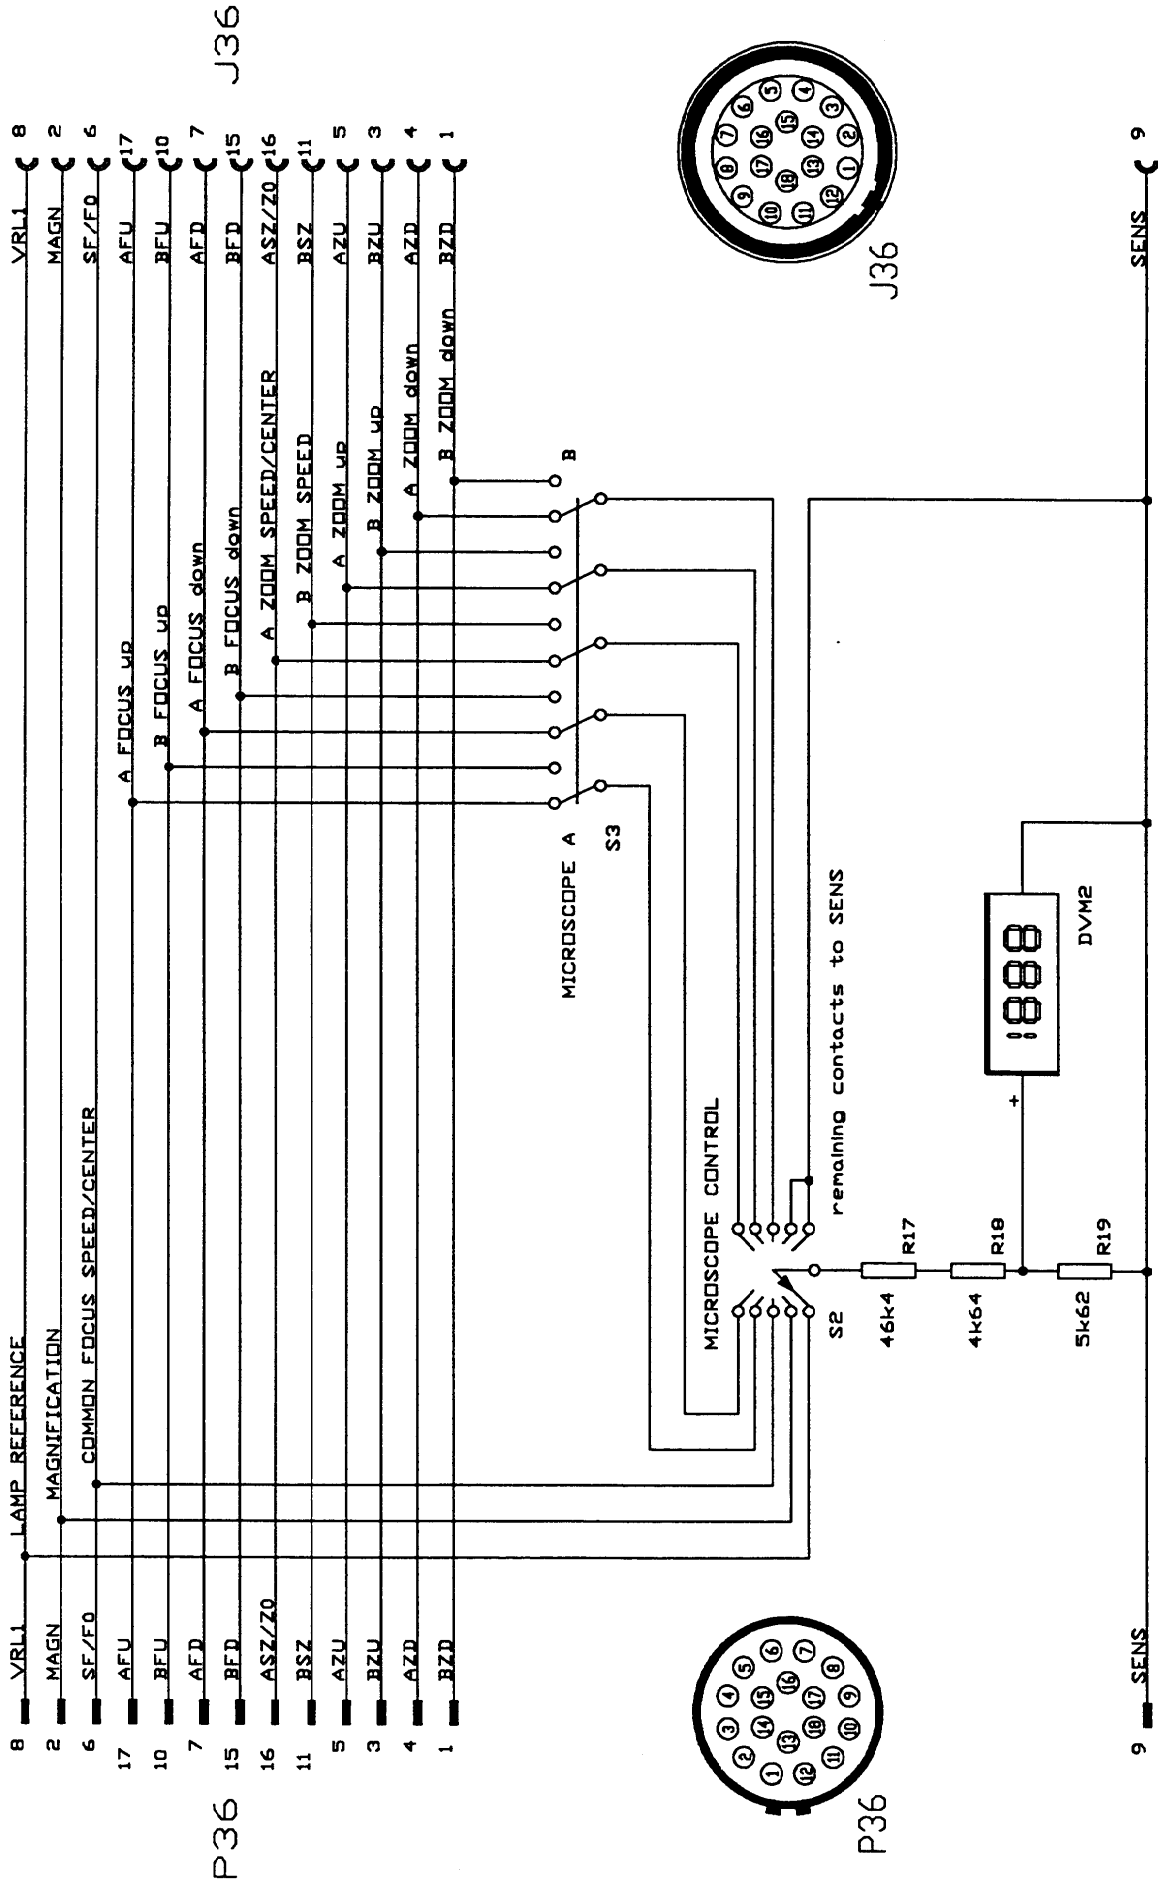


TESTBOX M695/680 - MICROSCOPE CONTROL

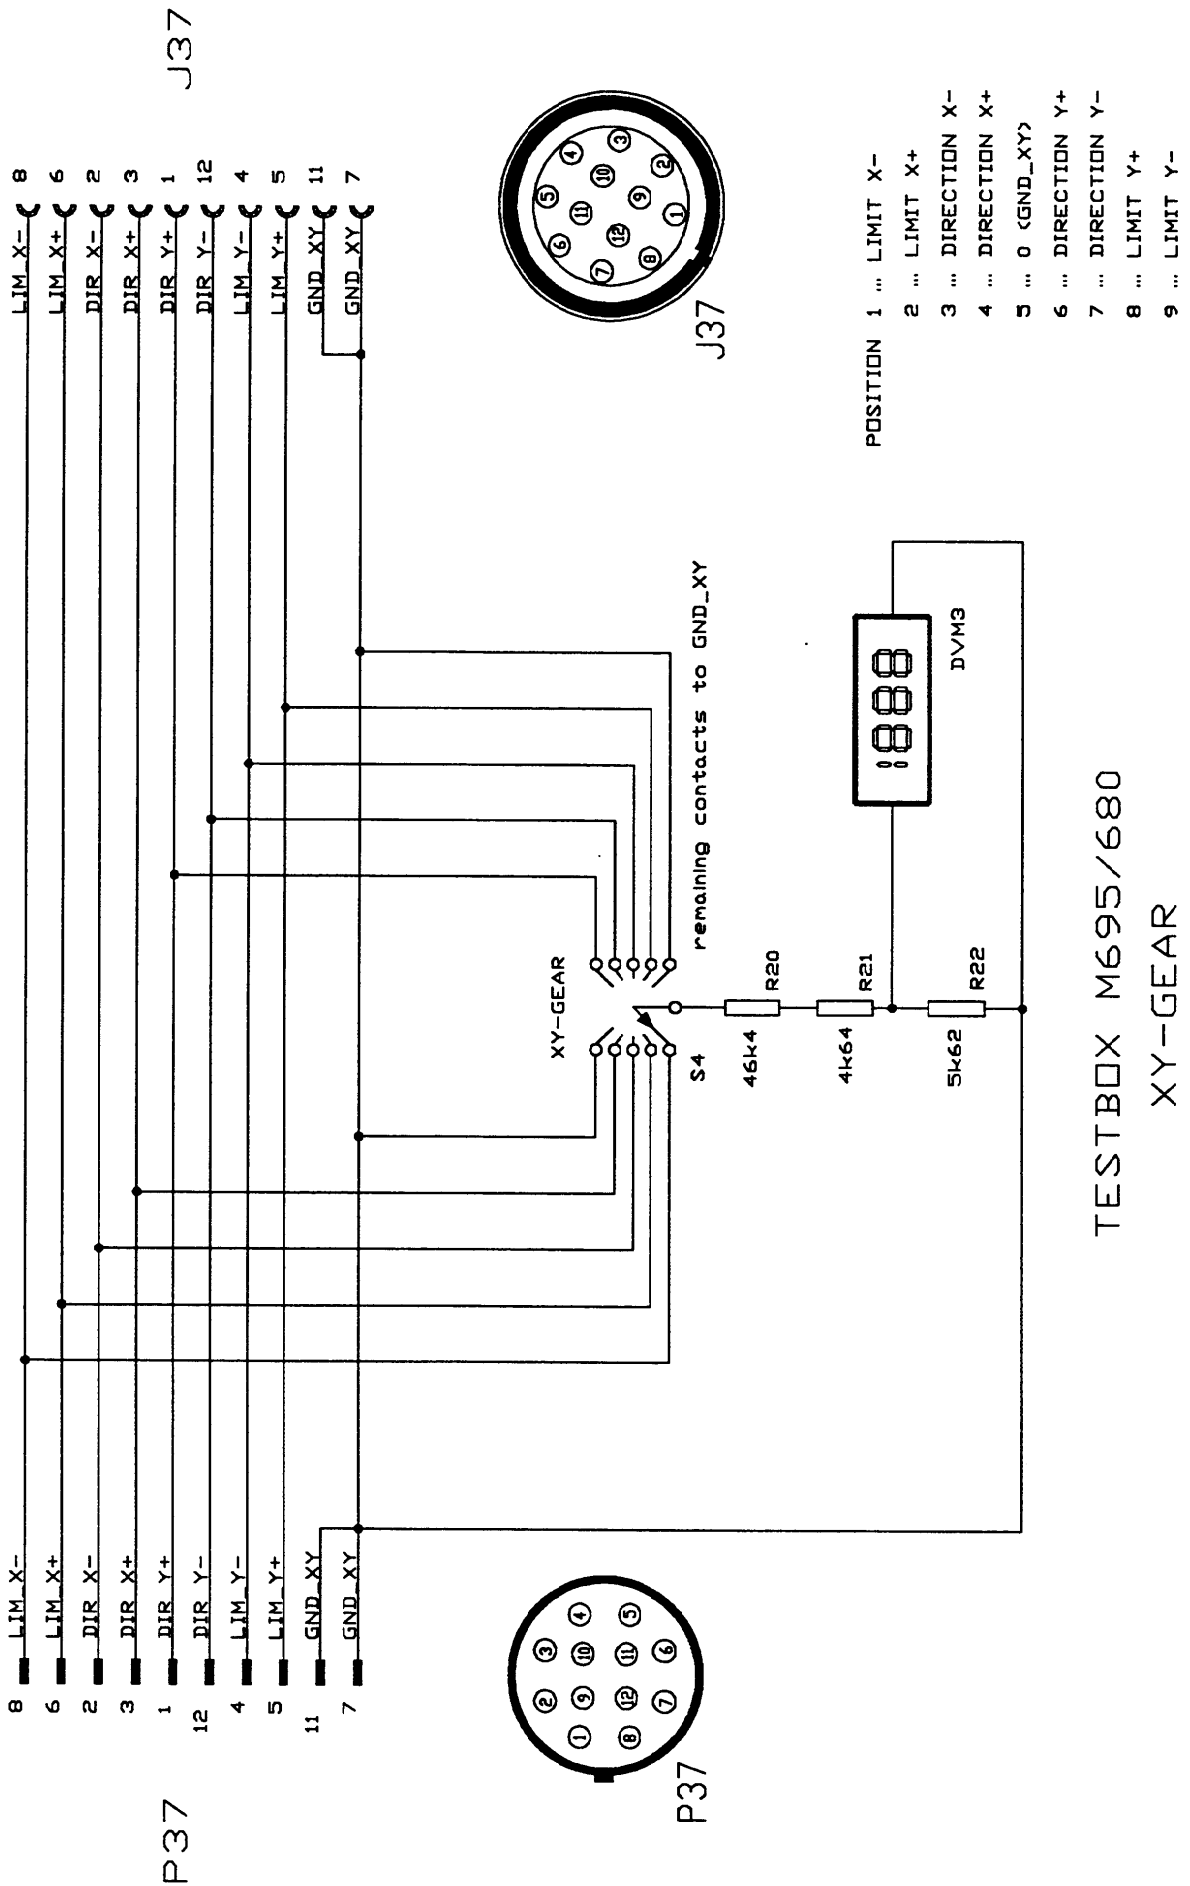

Service cable M695 / M680

for bridging the
swingarm

The service cable enables you to say whether the fault is in the control unit or in the swingarm.

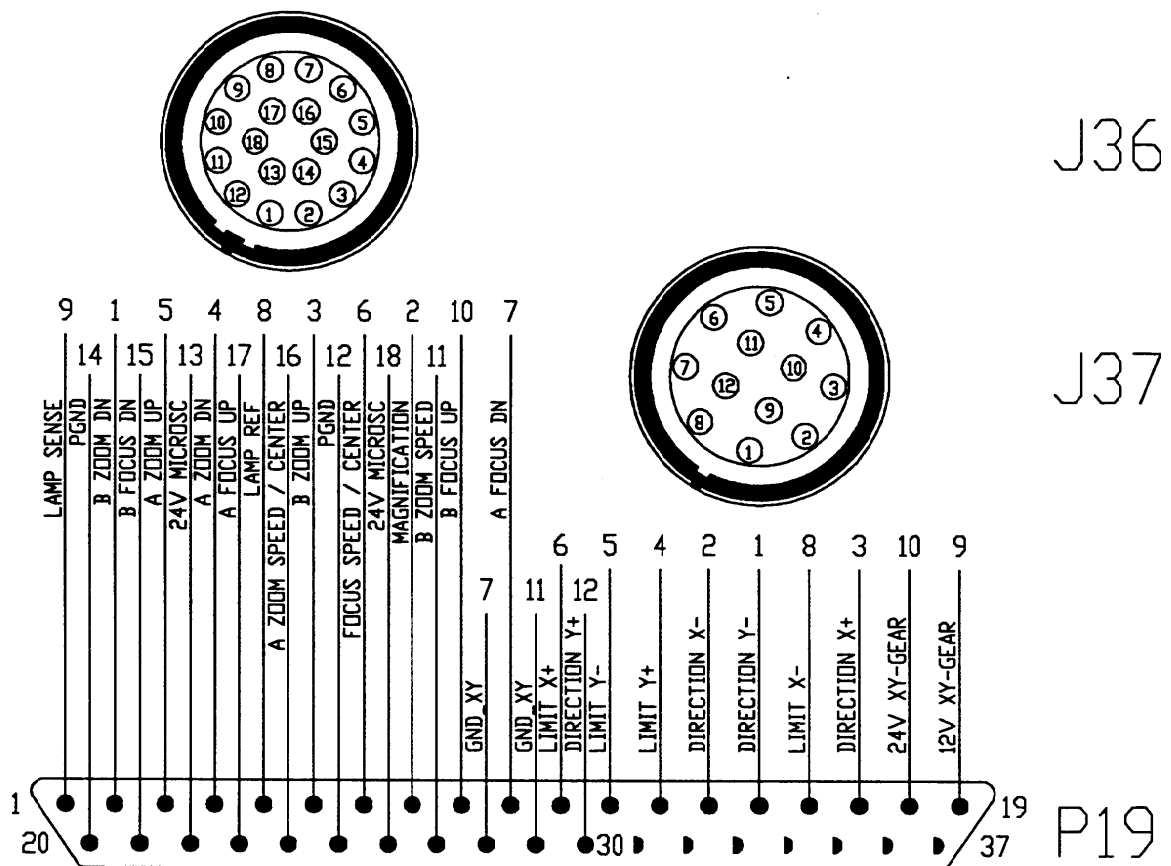

Art.Nr. Stock n°.	Benennung / Spezifikation Description / Specification	Bemerkung Remark	Zeichnung Drawing
----------------------	----------------------------------------------------------	---------------------	----------------------

Spare parts list M695

355 980 Lamp-control board

See page 11-2

Attention when the board is replaced at Instruments or with control units which are delivered since march 94: If the lamp control board does not have index C of modification or later it must be modified as shown on page 2-1.

Else the following fault occurs:
the hand-/footswitch at control input B does not react.

433 826 Gas spring

See page 10-4

507 990 Focus servo board

See page 11-1

526 770 Function display

Seepage 11-4

561 950 Panel hoard für MEL64/65

Seepage 11-3

567 930 Panel board für MEL61/62

See page 11-3

635 859 Swingarm cable

See page 10-5

635 972 Receiver board

See page 11-4


Art.Nr. Stock n°	Benennung / Spezifikation Description / Specification	Bemerkung Remark	Zeichnung Drawing
---------------------	----------------------------------------------------------	---------------------	----------------------




401 283 Pin spanner




418 135 Handle for pin spanner

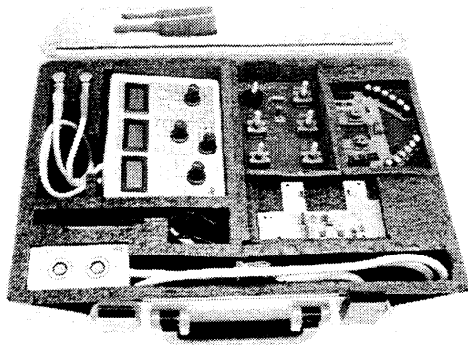


566 152 Test set compl. *without boards*

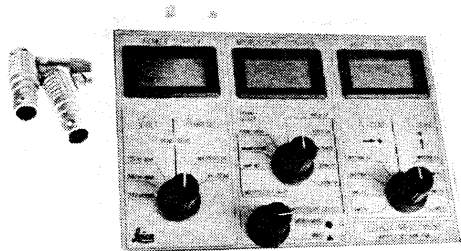

566 146 Test box

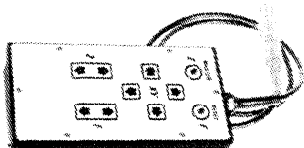

566 147 Hand switch mod.



556 148 Service cable (M680/M695)



566 151 Box

Free Manuals Download Website

<http://myh66.com>

<http://usermanuals.us>

<http://www.somanuals.com>

<http://www.4manuals.cc>

<http://www.manual-lib.com>

<http://www.404manual.com>

<http://www.luxmanual.com>

<http://aubethermostatmanual.com>

Golf course search by state

<http://golfingnear.com>

Email search by domain

<http://emailbydomain.com>

Auto manuals search

<http://auto.somanuals.com>

TV manuals search

<http://tv.somanuals.com>