

DAQ

PCI-6110E/6111E User Manual

Multifunction I/O Boards for

PCI Bus Computers

April 1998 Edition
Part Number 321759B-01

© Copyright 1998 National Instruments Corporation. All rights reserved.

Internet Support

E-mail: support@natinst.com

FTP Site: <ftp.natinst.com>

Web Address: <http://www.natinst.com>

Bulletin Board Support

BBS United States: 512 794 5422

BBS United Kingdom: 01635 551422

BBS France: 01 48 65 15 59

Fax-on-Demand Support

512 418 1111

Telephone Support (USA)

Tel: 512 795 8248

Fax: 512 794 5678

International Offices

Australia 03 9879 5166, Austria 0662 45 79 90 0, Belgium 02 757 00 20, Brazil 011 288 3336,
Canada (Ontario) 905 785 0085, Canada (Québec) 514 694 8521, Denmark 45 76 26 00,
Finland 09 725 725 11, France 01 48 14 24 24, Germany 089 741 31 30, Hong Kong 2645 3186,
Israel 03 6120092, Italy 02 413091, Japan 03 5472 2970, Korea 02 596 7456, Mexico 5 520 2635,
Netherlands 0348 433466, Norway 32 84 84 00, Singapore 2265886, Spain 91 640 0085, Sweden 08 730 49 70,
Switzerland 056 200 51 51, Taiwan 02 377 1200, United Kingdom 01635 523545

National Instruments Corporate Headquarters

6504 Bridge Point Parkway Austin, Texas 78730-5039 USA Tel: 512 794 0100

Important Information

Warranty

The PCI-6110E/6111E boards are warranted against defects in materials and workmanship for a period of one year from the date of shipment, as evidenced by receipts or other documentation. National Instruments will, at its option, repair or replace equipment that proves to be defective during the warranty period. This warranty includes parts and labor.

The media on which you receive National Instruments software are warranted not to fail to execute programming instructions, due to defects in materials and workmanship, for a period of 90 days from date of shipment, as evidenced by receipts or other documentation. National Instruments will, at its option, repair or replace software media that do not execute programming instructions if National Instruments receives notice of such defects during the warranty period. National Instruments does not warrant that the operation of the software shall be uninterrupted or error free.

A Return Material Authorization (RMA) number must be obtained from the factory and clearly marked on the outside of the package before any equipment will be accepted for warranty work. National Instruments will pay the shipping costs of returning to the owner parts which are covered by warranty.

National Instruments believes that the information in this manual is accurate. The document has been carefully reviewed for technical accuracy. In the event that technical or typographical errors exist, National Instruments reserves the right to make changes to subsequent editions of this document without prior notice to holders of this edition. The reader should consult National Instruments if errors are suspected. In no event shall National Instruments be liable for any damages arising out of or related to this document or the information contained in it.

EXCEPT AS SPECIFIED HEREIN, NATIONAL INSTRUMENTS MAKES NO WARRANTIES, EXPRESS OR IMPLIED, AND SPECIFICALLY DISCLAIMS ANY WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. CUSTOMER'S RIGHT TO RECOVER DAMAGES CAUSED BY FAULT OR NEGLIGENCE ON THE PART OF NATIONAL INSTRUMENTS SHALL BE LIMITED TO THE AMOUNT THEREFORE PAID BY THE CUSTOMER. NATIONAL INSTRUMENTS WILL NOT BE LIABLE FOR DAMAGES RESULTING FROM LOSS OF DATA, PROFITS, USE OF PRODUCTS, OR INCIDENTAL OR CONSEQUENTIAL DAMAGES, EVEN IF ADVISED OF THE POSSIBILITY THEREOF. This limitation of the liability of National Instruments will apply regardless of the form of action, whether in contract or tort, including negligence. Any action against National Instruments must be brought within one year after the cause of action accrues. National Instruments shall not be liable for any delay in performance due to causes beyond its reasonable control. The warranty provided herein does not cover damages, defects, malfunctions, or service failures caused by owner's failure to follow the National Instruments installation, operation, or maintenance instructions; owner's modification of the product; owner's abuse, misuse, or negligent acts; and power failure or surges, fire, flood, accident, actions of third parties, or other events outside reasonable control.

Copyright

Under the copyright laws, this publication may not be reproduced or transmitted in any form, electronic or mechanical, including photocopying, recording, storing in an information retrieval system, or translating, in whole or in part, without the prior written consent of National Instruments Corporation.

Trademarks

ComponentWorks™, CVI™, DAQ-STC™, LabVIEW™, Measure™, MITE™, NI-DAQ™, NI-PGIA™, RTSI™, SCXI™, and VirtualBench™ are trademarks of National Instruments Corporation.

Product and company names listed are trademarks or trade names of their respective companies.

WARNING REGARDING MEDICAL AND CLINICAL USE OF NATIONAL INSTRUMENTS PRODUCTS

National Instruments products are not designed with components and testing intended to ensure a level of reliability suitable for use in treatment and diagnosis of humans. Applications of National Instruments products involving medical or clinical treatment can create a potential for accidental injury caused by product failure, or by errors on the part of the user or application designer. Any use or application of National Instruments products for or involving medical or clinical treatment must be performed by properly trained and qualified medical personnel, and all traditional medical safeguards, equipment, and procedures that are appropriate in the particular situation to prevent serious injury or death should always continue to be used when National Instruments products are being used. National Instruments products are NOT intended to be a substitute for any form of established process, procedure, or equipment used to monitor or safeguard human health and safety in medical or clinical treatment.

*Table
of
Contents*

About This Manual

Organization of This Manual	xi
Conventions Used in This Manual	xii
National Instruments Documentation	xiii
Related Documentation	xiv
Customer Communication	xiv

Chapter 1

Introduction

About the 611X E Boards	1-1
What You Need to Get Started	1-2
Software Programming Choices	1-2
National Instruments Application Software	1-2
NI-DAQ Driver Software	1-3
Register-Level Programming	1-4
Optional Equipment	1-5
Custom Cabling	1-5
Unpacking	1-6

Chapter 2

Installation and Configuration

Software Installation	2-1
Hardware Installation	2-1
Board Configuration	2-2

Chapter 3

Hardware Overview

Analog Input	3-2
Input Mode	3-2
Input Polarity and Input Range	3-3
Considerations for Selecting Input Ranges	3-4
Input Coupling	3-4
Dither	3-4

Analog Output	3-5
Analog Trigger	3-6
Digital I/O.....	3-10
Timing Signal Routing	3-11
Programmable Function Inputs	3-12
Board and RTSI Clocks	3-12
RTSI Triggers	3-13

Chapter 4

Signal Connections

I/O Connector	4-1
I/O Connector Signal Descriptions	4-3
Analog Input Signal Connections.....	4-8
Types of Signal Sources	4-9
Floating Signal Sources	4-9
Ground-Referenced Signal Sources	4-9
Differential Measurements	4-9
Differential Connection Considerations.....	4-10
Differential Connections for Ground-Referenced Signal Sources	4-11
Differential Connections for Nonreferenced or Floating Signal Sources.....	4-11
Common-Mode Signal Rejection Considerations.....	4-12
Analog Output Signal Connections.....	4-13
Digital I/O Signal Connections	4-13
Power Connections.....	4-15
Timing Connections	4-15
Programmable Function Input Connections	4-16
DAQ Timing Connections	4-17
SCANCLK Signal	4-18
EXTSTROBE* Signal.....	4-18
TRIG1 Signal.....	4-19
TRIG2 Signal.....	4-20
STARTSCAN Signal.....	4-22
CONVERT* Signal	4-23
AIGATE Signal	4-25
SISOURCE Signal.....	4-25
Waveform Generation Timing Connections	4-26
WFTRIG Signal.....	4-26
UPDATE* Signal	4-27
UISOURCE Signal.....	4-28

General-Purpose Timing Signal Connections	4-29
GPCTR0_SOURCE Signal	4-29
GPCTR0_GATE Signal	4-30
GPCTR0_OUT Signal	4-31
GPCTR0_UP_DOWN Signal	4-31
GPCTR1_SOURCE Signal	4-32
GPCTR1_GATE Signal	4-32
GPCTR1_OUT Signal	4-33
GPCTR1_UP_DOWN Signal	4-34
FREQ_OUT Signal	4-35
Field Wiring Considerations	4-35

Chapter 5

Calibration

Loading Calibration Constants	5-1
Self-Calibration	5-2
External Calibration	5-2

Appendix A

Specifications

Appendix B

Cable Connector Descriptions

Appendix C

Common Questions

Appendix D

Customer Communication

Glossary

Index

Figures

Figure 1-1.	The Relationship between the Programming Environment, NI-DAQ, and Your Hardware	1-4
Figure 3-1.	PCI-6110E Block Diagram	3-1
Figure 3-2.	PCI-6111E Block Diagram	3-2
Figure 3-3.	Effects of Dither on Signal Acquisition	3-5
Figure 3-4.	Analog Trigger Block Diagram for the PCI-6110E	3-6
Figure 3-5.	Analog Trigger Block Diagram for the PCI-6111E	3-7
Figure 3-6.	Below-Low-Level Analog Triggering Mode	3-7
Figure 3-7.	Above-High-Level Analog Triggering Mode	3-8
Figure 3-8.	Inside-Region Analog Triggering Mode	3-8
Figure 3-9.	High-Hysteresis Analog Triggering Mode	3-9
Figure 3-10.	Low-Hysteresis Analog Triggering Mode	3-9
Figure 3-11.	CONVERT* Signal Routing	3-11
Figure 3-12.	RTSI Bus Signal Connection	3-13
Figure 4-1.	I/O Connector Pin Assignment for the 611X E Board	4-2
Figure 4-2.	611X E Board PGIA	4-8
Figure 4-3.	Differential Input Connections for Ground-Referenced Signals	4-11
Figure 4-4.	Differential Input Connections for Nonreferenced Signals	4-12
Figure 4-5.	Analog Output Connections	4-13
Figure 4-6.	Digital I/O Connections	4-14
Figure 4-7.	Timing I/O Connections	4-16
Figure 4-8.	Typical Posttriggered Acquisition	4-17
Figure 4-9.	Typical Pretriggered Acquisition	4-18
Figure 4-10.	SCANCLK Signal Timing	4-18
Figure 4-11.	EXTSTROBE* Signal Timing	4-19
Figure 4-12.	TRIG1 Input Signal Timing	4-20
Figure 4-13.	TRIG1 Output Signal Timing	4-20
Figure 4-14.	TRIG2 Input Signal Timing	4-21
Figure 4-15.	TRIG2 Output Signal Timing	4-21
Figure 4-16.	STARTSCAN Input Signal Timing	4-22
Figure 4-17.	STARTSCAN Output Signal Timing	4-23
Figure 4-18.	CONVERT* Input Signal Timing	4-24
Figure 4-19.	CONVERT* Output Signal Timing	4-24
Figure 4-20.	SISOURCE Signal Timing	4-26
Figure 4-21.	WFTRIG Input Signal Timing	4-27
Figure 4-22.	WFTRIG Output Signal Timing	4-27
Figure 4-23.	UPDATE* Input Signal Timing	4-28
Figure 4-24.	UPDATE* Output Signal Timing	4-28
Figure 4-25.	UISOURCE Signal Timing	4-29
Figure 4-26.	GPCTR0_SOURCE Signal Timing	4-30

Figure 4-27.	GPCTR0_GATE Signal Timing in Edge-Detection Mode	4-31
Figure 4-28.	GPCTR0_OUT Signal Timing	4-31
Figure 4-29.	GPCTR1_SOURCE Signal Timing	4-32
Figure 4-30.	GPCTR1_GATE Signal Timing in Edge-Detection Mode	4-33
Figure 4-31.	GPCTR1_OUT Signal Timing	4-33
Figure 4-32.	GPCTR Timing Summary	4-34
Figure B-1.	68-Pin 611X E Series Connector Pin Assignments	B-2

Tables

Table 3-1.	Actual Range and Measurement Precision	3-3
Table 4-1.	Signal Descriptions for I/O Connector Pins	4-3
Table 4-2.	I/O Signal Summary for the 611X E	4-6
Table 4-3.	Signal Source Types	4-10



*About
This
Manual*

This manual describes the electrical and mechanical aspects of the 611X E family of boards and contains information concerning their operation and programming.

The 611X E family of boards includes:

- PCI-6110E
- PCI-6111E

Your 611X E board is a high-performance multifunction analog, digital, and timing I/O board for PCI bus computers. Supported functions include analog input, analog output, digital I/O, and timing I/O.

Organization of This Manual



The *PCI-6110E/6111E User Manual* is organized as follows:

- **Chapter 1, *Introduction***, describes your 611X E board, lists what you need to get started, describes the optional software and optional equipment, and explains how to unpack your 611X E board.
- **Chapter 2, *Installation and Configuration***, explains how to install and configure your 611X E board.
- **Chapter 3, *Hardware Overview***, presents an overview of the hardware functions on your 611X E board.
- **Chapter 4, *Signal Connections***, describes how to make input and output signal connections to your 611X E board via the board I/O connector.
- **Chapter 5, *Calibration***, discusses the calibration procedures for your 611X E board.
- **Appendix A, *Specifications***, lists the specifications of your 611X E board.
- **Appendix B, *Cable Connector Descriptions***, describes the cable connectors on your 611X E board.

- [Appendix C, Common Questions](#), contains a list of commonly asked questions and their answers relating to usage and special features of your 611X E board.
- [Appendix D, Customer Communication](#), contains forms you can use to request help from National Instruments or to comment on our products.
- The [Glossary](#) contains an alphabetical list and description of terms used in this manual, including acronyms, abbreviations, definitions metric prefixes, mnemonics, and symbols.
- The [Index](#) alphabetically lists topics covered in this manual, including the page where you can find the topic.

Conventions Used in This Manual

The following conventions are used in this manual.

<>	Angle brackets enclose the name of a key on the keyboard (for example, <option>). Angle brackets containing numbers separated by an ellipsis represent a range of values associated with a bit or signal name (for example, DIO<3..0>).
611X E	This refers to either the PCI-6110E or PCI-6111E board.
	This icon to the left of bold italicized text denotes a note, which alerts you to important information.
	This icon to the left of bold italicized text denotes a caution, which advises you of precautions to take to avoid injury, data loss, or a system crash.
bold	Bold text denotes the names of menus, menu items, parameters, dialog boxes, dialog box buttons or options, icons, windows, Windows 95 tabs, or LEDs.
<i>bold italic</i>	Bold italic text denotes a note, caution, or warning.
<i>italic</i>	Italic text denotes emphasis, a cross reference, or an introduction to a key concept. This font also denotes text from which you supply the appropriate word or value, as in Windows 3.x.
Macintosh	Macintosh refers to all Macintosh OS computers with PCI bus, unless otherwise noted.

monospace	Text in this font denotes text or characters that you should literally enter from the keyboard, sections of code, programming examples, and syntax examples. This font also is used for the proper names of disk drives, paths, directories, programs, subprograms, subroutines, device names, functions, operations, variables, filenames, and extensions, and for statements and comments taken from program code.
NI-DAQ	NI-DAQ refers to the NI-DAQ driver software for Macintosh or PC compatible computers unless otherwise noted.
PC	Refers to all PC AT series computers with PCI bus unless otherwise noted.
SCXI	SCXI stands for Signal Conditioning eXtensions for Instrumentation and is a National Instruments product line designed to perform front-end signal conditioning for National instruments plug-in DAQ boards.

National Instruments Documentation

The *PCI-6110E/6111E User Manual* is one piece of the documentation set for your DAQ system. You could have any of several types of documentation depending on the hardware and software in your system. Use the documentation you have as follows:

- *Getting Started with SCXI*—If you are using SCXI, this is the first manual you should read. It gives an overview of the SCXI system and contains the most commonly needed information for the modules, chassis, and software.
- Your SCXI hardware user manuals—If you are using SCXI, read these manuals next for detailed information about signal connections and module configuration. They also explain in greater detail how the module works and contain application hints.
- Your DAQ hardware documentation—This documentation has detailed information about the DAQ hardware that plugs into or is connected to your computer. Use this documentation for hardware installation and configuration instructions, specification information about your DAQ hardware, and application hints.
- Software documentation—You may have both application software and NI-DAQ software documentation. National Instruments application software includes ComponentWorks, LabVIEW, LabWindows/CVI, Measure, and VirtualBench. After you set up your hardware system, use either your application software

documentation or the NI-DAQ documentation to help you write your application. If you have a large, complicated system, it is worthwhile to look through the software documentation before you configure your hardware.

- Accessory installation guides or manuals—If you are using accessory products, read the terminal block and cable assembly installation guides. They explain how to physically connect the relevant pieces of the system. Consult these guides when you are making your connections.
- SCXI chassis manuals—If you are using SCXI, read these manuals for maintenance information on the chassis and installation instructions.

Related Documentation

The following documents contain information you may find helpful:

- *DAQ-STC Technical Reference Manual*
- National Instruments Application Note 025, *Field Wiring and Noise Considerations for Analog Signals*
- *PCI Local Bus Specification Revision 2.0*

Customer Communication

National Instruments wants to receive your comments on our products and manuals. We are interested in the applications you develop with our products, and we want to help if you have problems with them. To make it easy for you to contact us, this manual contains comment and configuration forms for you to complete. These forms are in [Appendix D, *Customer Communication*](#), at the end of this manual.

Introduction

Chapter

1

This chapter describes your 611X E board, lists what you need to get started, describes the optional software and optional equipment, and explains how to unpack your 611X E board.

About the 611X E Boards

Thank you for buying a National Instruments PCI-6110E/6111E board. Your 611X E board is a completely Plug and Play, multifunction analog, digital, and timing I/O board for PCI bus computers. The 611X E board features a 12-bit ADC per channel with four or two simultaneously sampling analog inputs, 16-bit DACs with voltage outputs, eight lines of TTL-compatible digital I/O, and two 24-bit counter/timers for timing I/O. Because the 611X E board has no DIP switches, jumpers, or potentiometers, it is easily software-configured and calibrated.

The 611X E board is a completely switchless and jumperless data acquisition (DAQ) board for the PCI bus. This feature is made possible by the National Instruments MITE bus interface chip that connects the board to the PCI I/O bus. The MITE implements the PCI Local Bus Specification so that the interrupts and base memory addresses are all software configured.

The 611X E board uses the National Instruments DAQ-STC system timing controller for time-related functions. The DAQ-STC consists of three timing groups that control analog input, analog output, and general-purpose counter/timer functions. These groups include a total of seven 24-bit and three 16-bit counters and a maximum timing resolution of 50 ns. The DAQ-STC makes possible such applications as buffered pulse generation, equivalent time sampling, and seamlessly changing the sampling rate.

Often with DAQ boards, you cannot easily synchronize several measurement functions to a common trigger or timing event. The 611X E board has the Real-Time System Integration (RTSI) bus to solve this problem. The RTSI bus consists of our RTSI bus interface

and a ribbon cable to route timing and trigger signals between several functions on as many as five DAQ boards in your computer.

Detailed specifications of the 611X E board are in Appendix A, *Specifications*.

What You Need to Get Started

To set up and use the 611X E board, you will need the following:

- Either the PCI-6110E or PCI-6111E board
- PCI-6110E/6111E User Manual*
- One of the following software packages and documentation:
 - ComponentWorks
 - LabVIEW for Macintosh
 - LabVIEW for Windows
 - LabWindows/CVI for Windows
 - Measure
 - NI-DAQ for PC Compatibles
 - VirtualBench
- Your computer

Software Programming Choices

You have several options to choose from when programming your National Instruments DAQ and SCXI hardware. You can use National Instruments application software, NI-DAQ, or register-level programming.

National Instruments Application Software

ComponentWorks contains tools for data acquisition and instrument control built on NI-DAQ driver software. ComponentWorks provides a higher-level programming interface for building virtual instruments through standard OLE controls and DLLs. With ComponentWorks, you can use all of the configuration tools, resource management utilities, and interactive control utilities included with NI-DAQ.

LabVIEW features interactive graphics, a state-of-the-art user interface, and a powerful graphical programming language. The

LabVIEW Data Acquisition VI Library, a series of VIs for using LabVIEW with National Instruments DAQ hardware, is included with LabVIEW. The LabVIEW Data Acquisition VI Library is functionally equivalent to NI-DAQ software.

LabWindows/CVI features interactive graphics, state-of-the-art user interface, and uses the ANSI standard C programming language. The LabWindows/CVI Data Acquisition Library, a series of functions for using LabWindows/CVI with National Instruments DAQ hardware, is included with the NI-DAQ software kit. The LabWindows/CVI Data Acquisition Library is functionally equivalent to the NI-DAQ software.

VirtualBench features virtual instruments that combine DAQ products, software, and your computer to create a stand-alone instrument with the added benefit of the processing, display, and storage capabilities of your computer. VirtualBench instruments load and save waveform data to disk in the same forms that can be used in popular spreadsheet programs and word processors.

Using ComponentWorks, LabVIEW, LabWindows/CVI, or VirtualBench software will greatly reduce the development time for your data acquisition and control application.

NI-DAQ Driver Software

The NI-DAQ driver software is included at no charge with all National Instruments DAQ hardware. NI-DAQ is not packaged with SCXI or accessory products, except for the SCXI-1200. NI-DAQ has an extensive library of functions that you can call from your application programming environment. These functions include routines for analog input (A/D conversion), buffered data acquisition (high-speed A/D conversion), analog output (D/A conversion), waveform generation (timed D/A conversion), digital I/O, counter/timer operations, SCXI, RTSI, self-calibration, messaging, and acquiring data to extended memory.

NI-DAQ has both high-level DAQ I/O functions for maximum ease of use and low-level DAQ I/O functions for maximum flexibility and performance. Examples of high-level functions are streaming data to disk or acquiring a certain number of data points. An example of a low-level function is writing directly to registers on the DAQ device. NI-DAQ does not sacrifice the performance of National Instruments DAQ devices because it lets multiple devices operate at their peak.

NI-DAQ also internally addresses many of the complex issues between the computer and the DAQ hardware such as programming interrupts and DMA controllers. NI-DAQ maintains a consistent software interface among its different versions so that you can change platforms with minimal modifications to your code. Whether you are using conventional programming languages or National Instruments application software, your application uses the NI-DAQ driver software, as illustrated in Figure 1-1.

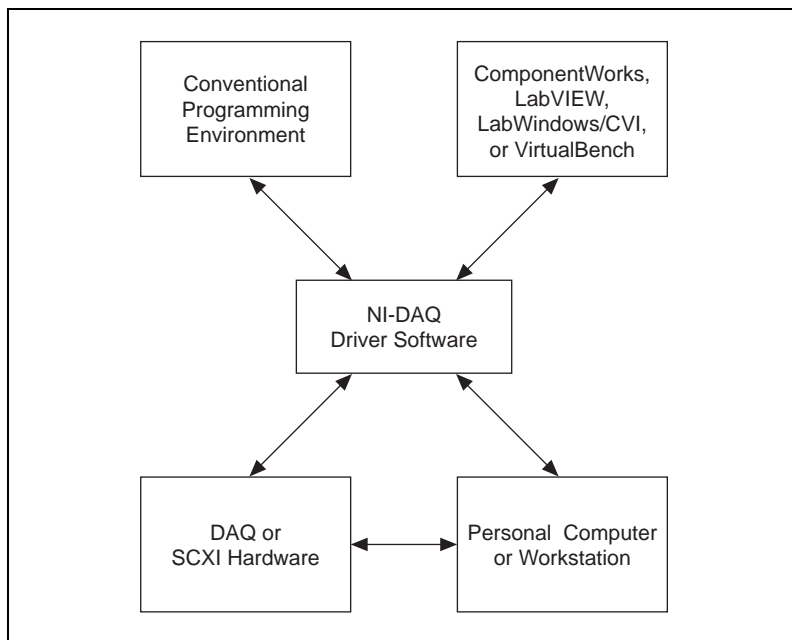


Figure 1-1. The Relationship between the Programming Environment, NI-DAQ, and Your Hardware

Register-Level Programming

The final option for programming any National Instruments DAQ hardware is to write register-level software. Writing register-level programming software can be very time-consuming and inefficient, and is not recommended for most users.

Even if you are an experienced register-level programmer, using NI-DAQ or application software to program your National Instruments DAQ hardware is easier than, and as flexible as, register-level programming, and can save weeks of development time.

Optional Equipment

National Instruments offers a variety of products to use with the 611X E board, including cables, connector blocks, and other accessories, as follows:

- Cables and cable assemblies
- Connector blocks, shielded and unshielded 50- and 68-pin screw terminals
- RTSI bus cables
- Low channel-count signal conditioning modules, boards, and accessories, including conditioning for strain gauges, RTDs, and relays

For more specific information about these products, refer to your National Instruments catalogue or call the office nearest you.

Custom Cabling

National Instruments offers cables and accessories for you to prototype your application or to use if you frequently change board interconnections.

If you want to develop your own cable, however, the following guidelines may be useful:

- For the analog input signals, shielded twisted-pair wires for each analog input pair yield the best results, assuming that you use differential inputs. Tie the shield for each signal pair to the ground reference at the source.
- Route the analog lines separately from the digital lines.
- When using a cable shield, use separate shields for the analog and digital halves of the cable. Failure to do so results in noise coupling into the analog signals from transient digital signals.

Mating connectors and a backshell kit for making custom 68-pin cables are available from National Instruments.

The following list gives recommended part numbers for connectors that mate to the I/O connector on the 611X E board:


- Honda 68-position, solder cup, female connector (part number PCS-E68FS)
- Honda backshell (part number PCS-E68LKPA)

Unpacking

The 611X E board is shipped in an antistatic package to prevent electrostatic damage to the board. Electrostatic discharge can damage several components on the board. To avoid such damage in handling the board, take the following precautions:

- Ground yourself via a grounding strap or by holding a grounded object.
- Touch the antistatic package to a metal part of your computer chassis before removing the board from the package.
- Remove the board from the package and inspect the board for loose components or any other sign of damage. Notify National Instruments if the board appears damaged in any way. Do *not* install a damaged board into your computer.
- *Never* touch the exposed pins of connectors.

Installation and Configuration

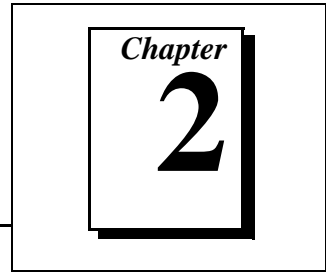

This chapter explains how to install and configure your 611X E board.

Software Installation

Install your software before you install the 611X E board. Refer to the appropriate release notes indicated below for specific instructions on the software installation sequence.

If you are using LabVIEW, LabWindows/CVI, or other National Instruments application software packages, refer to the appropriate release notes. After you have installed your application software, refer to your NI-DAQ release notes and follow the instructions given there for your operating system and application software package.

If you are using NI-DAQ, refer to your NI-DAQ release notes. Find the installation section for your operating system and follow the instructions given there.

Hardware Installation

You can install the 611X E board in any available expansion slot in your computer. However, to achieve best noise performance, leave as much room as possible between the 611X E board and other boards and hardware. The following are general installation instructions, but consult your computer user manual or technical reference manual for specific instructions and warnings.

1. Write down the 611X E board serial number in the *PCI-6110E/6111E Hardware and Software Configuration Form* in *Appendix D, Customer Communication*, of this manual.
2. Turn off and unplug your computer.
3. Remove the top cover or access port to the I/O channel.
4. Remove the expansion slot cover on the back panel of the computer.

5. Insert the 611X E board into a 5 V PCI slot. Gently rock the board to ease it into place. It may be a tight fit, but *do not force* the board into place.
6. If required, screw the mounting bracket of the 611X E board to the back panel rail of the computer.
7. Replace the cover.
8. Plug in and turn on your computer.

The 611X E board is installed. You are now ready to configure your software. Refer to your software documentation for configuration instructions.

Board Configuration

Due to the National Instruments standard architecture for data acquisition and the PCI bus specification, the 611X E board is completely software configurable. You must perform two types of configuration on the 611X E board—bus-related and data acquisition-related configuration.

The 611X E board is fully compatible with the industry standard *PCI Local Bus Specification Revision 2.0*. This allows the PCI system to automatically perform all bus-related configurations and requires no user interaction. Bus-related configuration includes setting the board base memory address and interrupt channel.

Data acquisition-related configuration includes such settings as analog input coupling and range, and others. You can modify these settings using NI-DAQ or application level software, such as ComponentWorks, LabVIEW, LabWindows/CVI, and VirtualBench.

Hardware Overview

This chapter presents an overview of the hardware functions on your 611X E board. Figure 3-1 shows a block diagram for the PCI-6110E board.

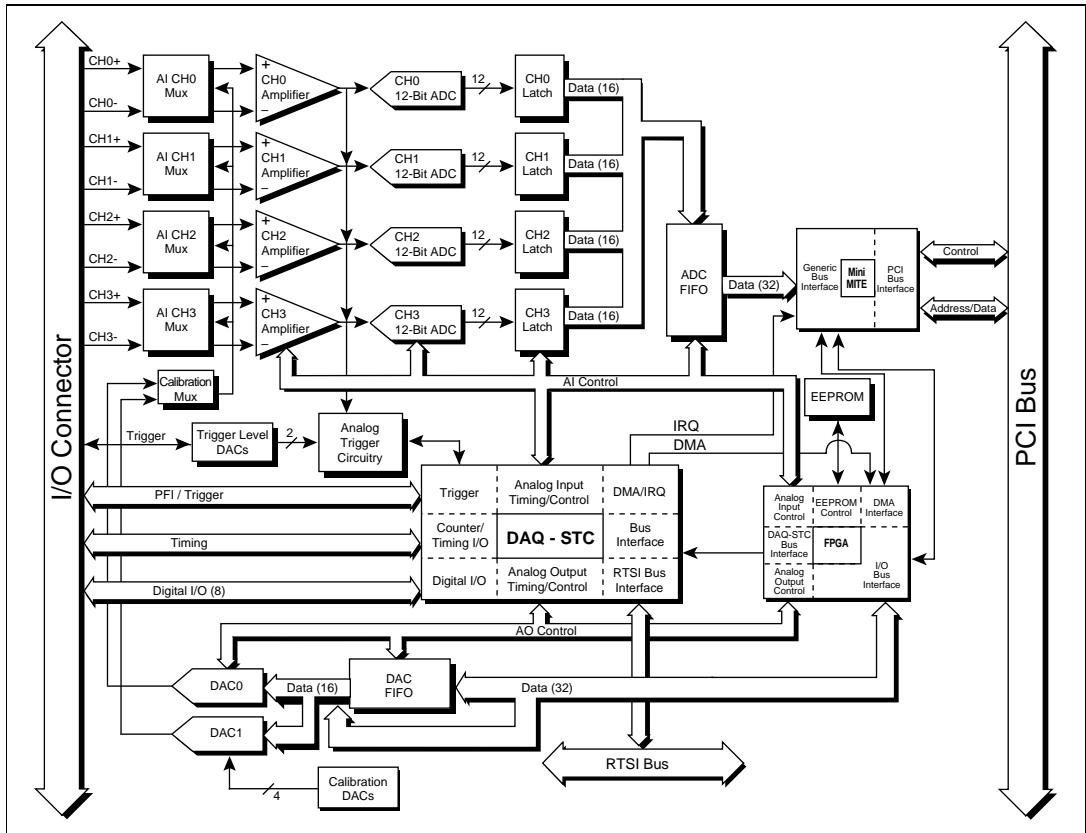


Figure 3-1. PCI-6110E Block Diagram

Figure 3-2 shows a block diagram for the PCI-6111E board.

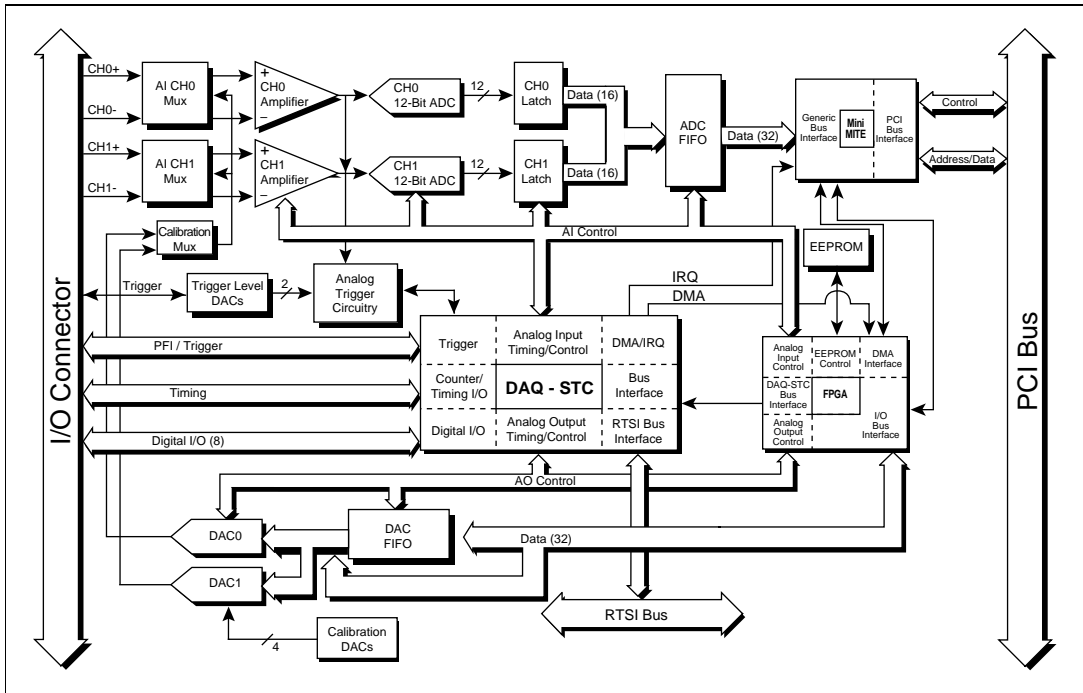


Figure 3-2. PCI-6111E Block Diagram

Analog Input

The analog input section for the 611X E board is software configurable. You can select different analog input configurations through application software. The following sections describe in detail each of the analog input categories.

Input Mode

The 611X E board supports only differential inputs (DIFF). The DIFF input configuration provides up to four channels on the PCI-6110E board and up to two channels on the PCI-6111E board.

A channel configured in DIFF mode uses two analog channel input lines. One line connects to the positive input of the board programmable gain instrumentation amplifier (PGIA), and the other connects to the negative input of the PGIA. For more information about DIFF input

configuration, refer to the *Analog Input Signal Connections* section in Chapter 4, *Signal Connections*, which contains diagrams showing the signal paths for DIFF input.

Input Polarity and Input Range

The 611X E board has bipolar inputs only. Bipolar input means that the input voltage range is between $-V_{\text{ref}}/2$ and $+V_{\text{ref}}/2$. These boards have a bipolar input range of 20 V (± 10 V).

You can program range settings on a per channel basis so that you can configure each input channel uniquely.

The software-programmable gain on these boards increases their overall flexibility by matching the input signal ranges to those that the ADC can accommodate. They have gains of 0.2, 0.5, 1, 2, 5, 10, 20, and 50, and are suited for a wide variety of signal levels. With the proper gain setting, you can use the full resolution of the ADC to measure the input signal. Table 3-1 shows the overall input range and precision according to the gain used.

Table 3-1. Actual Range and Measurement Precision

Range Configuration	Gain	Actual Input Range ¹	Precision ²
-10 to +10 V	0.2	-50 to +50 V	24.41 mV
	0.5	-20 to +20 V	9.77 mV
	1.0	-10 to +10 V	4.88 mV
	2.0	-5 to +5 V	2.44 mV
	5.0	-2 to +2 V	976.56 μ V
	10.0	-1 to +1 V	488.28 μ V
	20.0	-500 to +500 mV	244.14 μ V
	50.0	-200 to +200 mV	97.66 μ V

¹ **Warning:** The 611X E is not designed for input voltages greater than 42 V, even if a user-installed voltage divider reduces the voltage to within the input range of the DAQ device. Input voltages greater than 42 V can damage the 611X E, any device connected to it, and the host computer. Overvoltage can also cause an electric shock hazard for the operator. National Instruments is NOT liable for damage or injury resulting from such misuse.

² The value of 1 LSB of the 12-bit ADC; that is, the voltage increment corresponding to a change of one count in the ADC 12-bit count.

Note: See Appendix A, *Specifications*, for absolute maximum ratings.

Considerations for Selecting Input Ranges

The range you select depends on the expected range of the incoming signal. A large input range can accommodate a large signal variation but reduces the voltage resolution. Choosing a smaller input range improves the voltage resolution but may result in the input signal going out of range. For best results, match the input range as closely as possible to the expected range of the input signal.

Input Coupling

You can configure the 611XE board for either AC or DC input coupling on a per channel basis. Use AC coupling when your AC signal contains a large DC component. If you enable AC coupling, you remove the large DC offset for the input amplifier and amplify only the AC component. This makes effective use of the ADC dynamic range.

Dither

Dither adds approximately 0.5 LSB_{rms} of white Gaussian noise to the signal to be converted by the ADC. This addition is useful for applications involving averaging to increase the resolution of the 611XE board, as in calibration or spectral analysis. In such applications, noise modulation is decreased and differential linearity is improved by the addition of the dither. When taking DC measurements, such as when checking the board calibration, you should average about 1,000 points to take a single reading. This process removes the effects of quantization and reduces measurement noise, resulting in improved resolution.

Figure 3-3 illustrates the effect of dither on signal acquisition. Figure 3-3a shows a small (± 4 LSB) sine wave acquired without dither. The ADC quantization is clearly visible. Figure 3-3b shows what happens when 50 such acquisitions are averaged together; quantization is still plainly visible. In Figure 3-3c, the sine wave is acquired with dither. There is a considerable amount of visible noise. But averaging about 50 such acquisitions, as shown in Figure 3-3d, eliminates both the added noise and the effects of quantization. Dither has the effect of forcing quantization noise to become a zero-mean random variable rather than a deterministic function of the input signal.

You cannot disable dither on the 611X E board. This is because the ADC resolution is so fine that the ADC and the PGIA inherently produce almost 0.5 LSBrms of noise. This is equivalent to having a dither circuit that is always enabled.

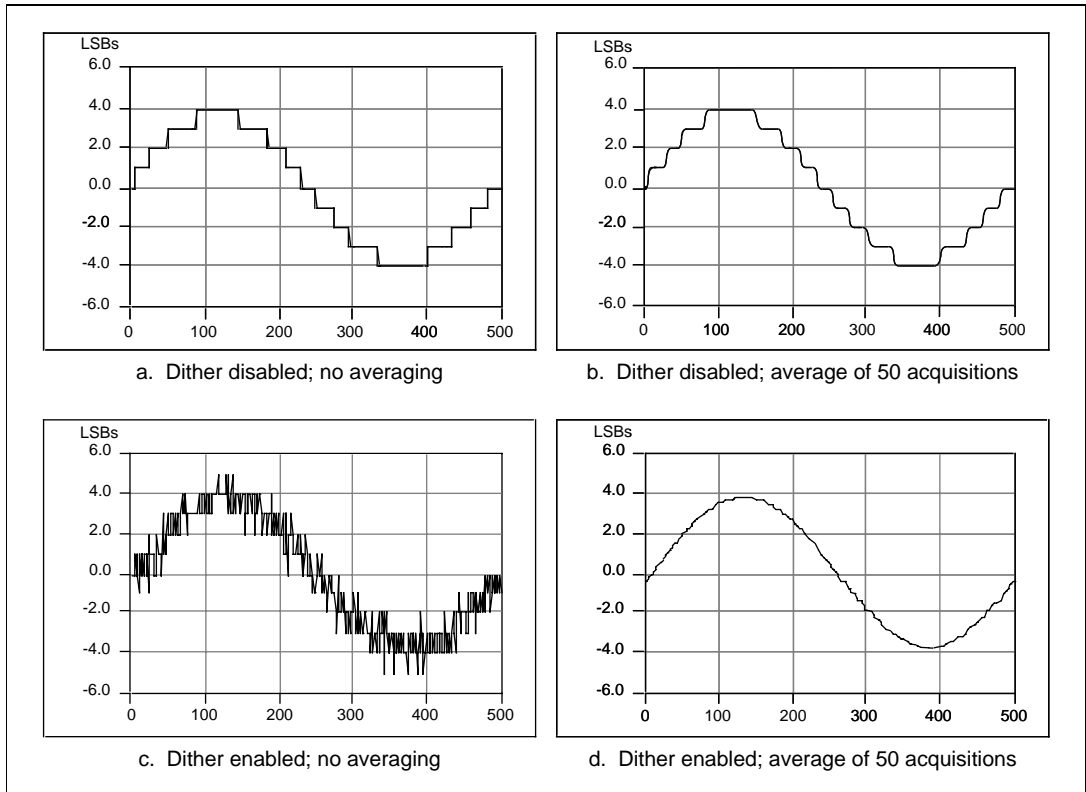


Figure 3-3. Effects of Dither on Signal Acquisition

Analog Output

The 611X E board supplies two channels of analog output voltage at the I/O connector. The range is fixed at bipolar ± 10 V.

Analog Trigger

In addition to supporting internal software triggering and external digital triggering to initiate a data acquisition sequence, these boards also support analog triggering. You can configure the analog trigger circuitry to accept either a direct analog input from the PFI0/TRIG1 pin on the I/O connector or a postgain signal from the output of the PGIA on any of the channels, as shown in Figures 3-4 and 3-5. The trigger-level range for the direct analog channel is ± 10 V in 78 mV steps for the 611X E board. The range for the post-PGIA trigger selection is simply the full-scale range of the selected channel, and the resolution is that range divided by 256.



Note:

The PFI0/TRIG1 pin is an analog input when configured as an analog trigger. Therefore, it is susceptible to crosstalk from adjacent pins, which can result in false triggering when the pin is left unconnected. To avoid false triggering, make sure this pin is connected to a low-impedance signal source (less than 1 k Ω source impedance) if you plan to enable this input via software.

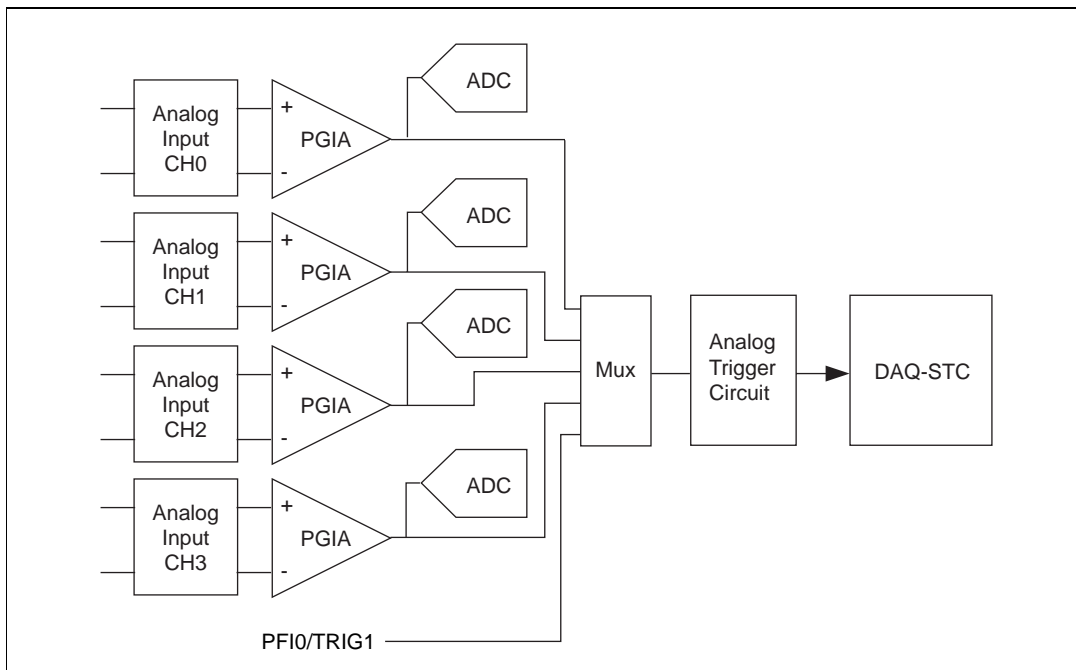


Figure 3-4. Analog Trigger Block Diagram for the PCI-6110E

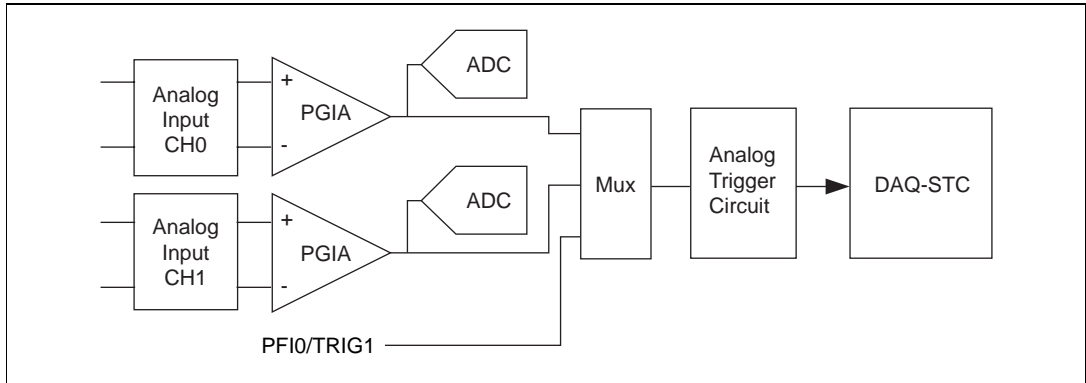


Figure 3-5. Analog Trigger Block Diagram for the PCI-6111E

Five analog triggering modes are available, as shown in Figures 3-6 through 3-10. You can set **lowValue** and **highValue** independently in software.

In below-low-level analog triggering mode, the trigger is generated when the signal value is less than **lowValue**, as shown in Figure 3-6. **HighValue** is unused.

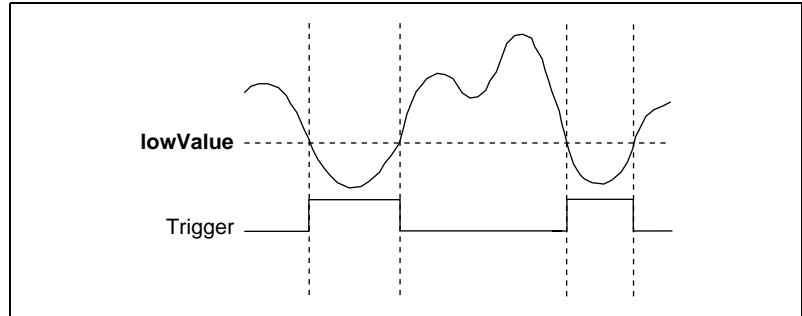


Figure 3-6. Below-Low-Level Analog Triggering Mode

In above-high-level analog triggering mode, the trigger is generated when the signal value is greater than **highValue**, as shown in Figure 3-7. **LowValue** is unused.

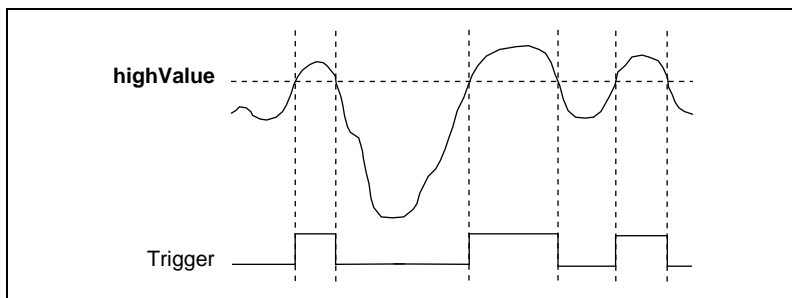


Figure 3-7. Above-High-Level Analog Triggering Mode

In inside-region analog triggering mode, the trigger is generated when the signal value is between the **lowValue** and the **highValue**, as shown in Figure 3-8.

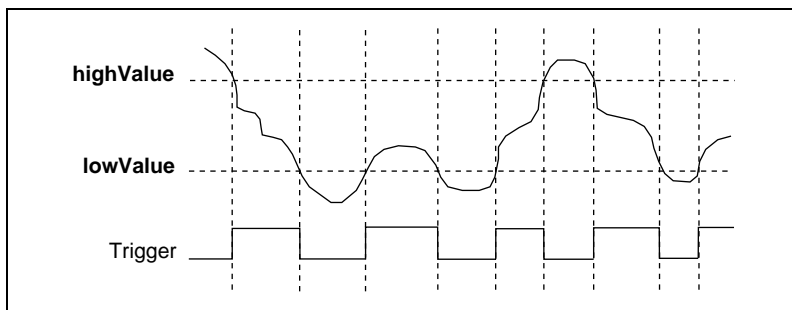


Figure 3-8. Inside-Region Analog Triggering Mode

In high-hysteresis analog triggering mode, the trigger is generated when the signal value is greater than **highValue**, with the hysteresis specified by **lowValue**, as shown in Figure 3-9.

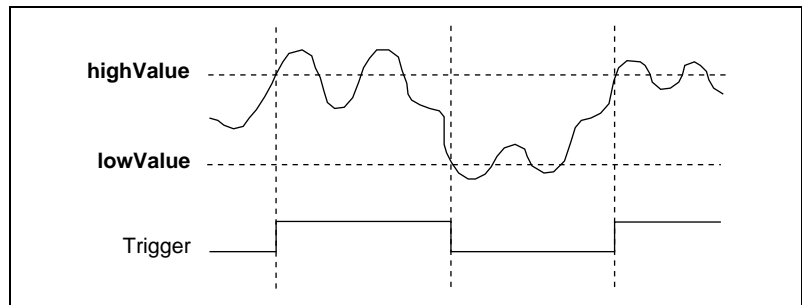


Figure 3-9. High-Hysteresis Analog Triggering Mode

In low-hysteresis analog triggering mode, the trigger is generated when the signal value is less than **lowValue**, with the hysteresis specified by **highValue**, as shown in Figure 3-10.

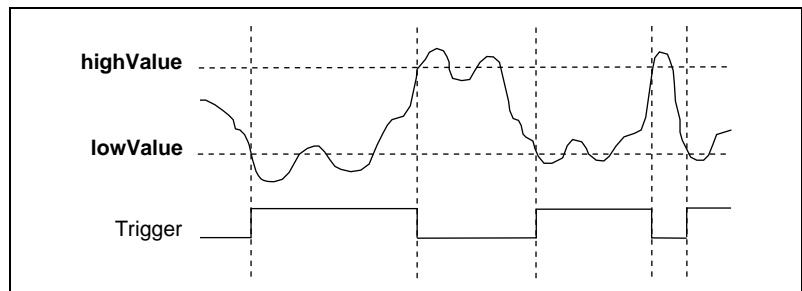


Figure 3-10. Low-Hysteresis Analog Triggering Mode

The analog trigger circuit generates an internal digital trigger based on the analog input signal and the user-defined trigger levels. This digital trigger can be used by any of the timing sections of the DAQ-STC, including the analog input, analog output, and general-purpose counter/timer sections. For example, the analog input section can be configured to acquire n scans after the analog input signal crosses a specific threshold. As another example, the analog output section can be configured to update its outputs whenever the analog input signal crosses a specific threshold.

Digital I/O

The 611XE board contains eight lines of digital I/O for general-purpose use. You can individually software-configure each line for either input or output. At system startup and reset, the digital I/O ports are all high impedance.

The hardware up/down control for general-purpose counters 0 and 1 are connected onboard to DIO6 and DIO7, respectively. Thus, you can use DIO6 and DIO7 to control the general-purpose counters. The up/down control signals are input only and do not affect the operation of the DIO lines.

Timing Signal Routing

The DAQ-STC provides a very flexible interface for connecting timing signals to other boards or external circuitry. The 611X E board uses the RTSI bus to interconnect timing signals between boards, and the Programmable Function Input (PFI) pins on the I/O connector to connect the board to external circuitry. These connections are designed to enable the 611X E board to both control and be controlled by other boards and circuits.

There are a total of 13 timing signals internal to the DAQ-STC that can be controlled by an external source. These timing signals can also be controlled by signals generated internally to the DAQ-STC, and these selections are fully software configurable. For example, the signal routing multiplexer for controlling the CONVERT* signal is shown in Figure 3-11.

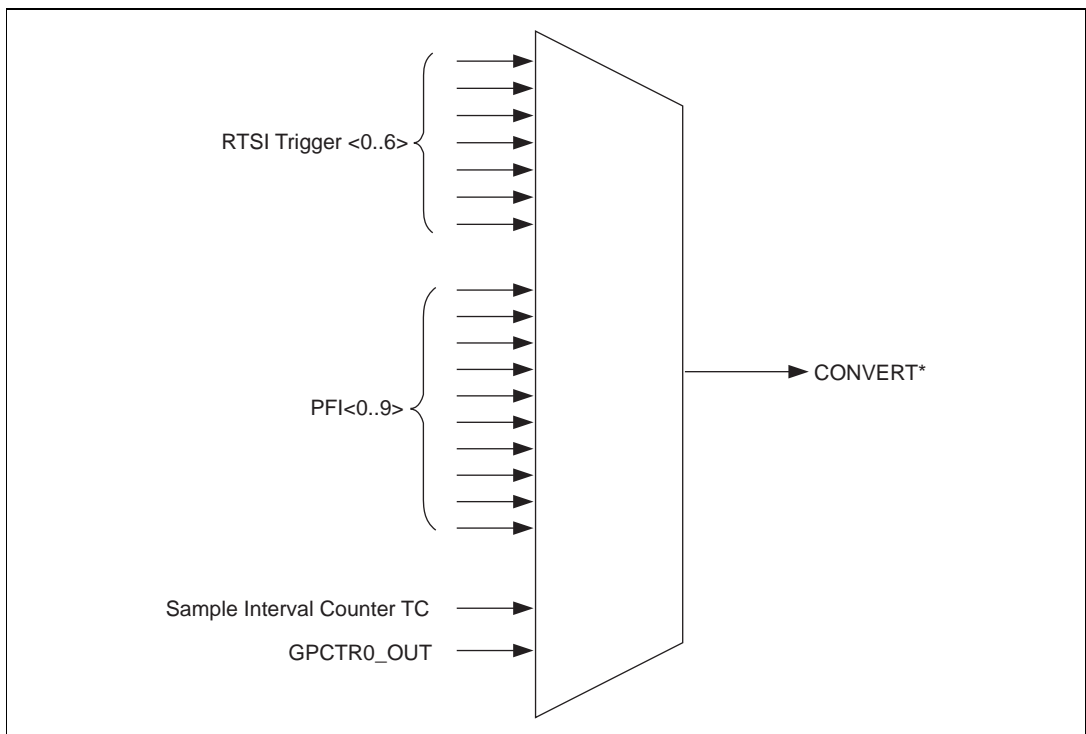


Figure 3-11. CONVERT* Signal Routing

This figure shows that CONVERT* can be generated from a number of sources, including the external signals RTSI<0..6> and PFI<0..9> and the internal signals Sample Interval Counter TC and GPCTR0_OUT.

Many of these timing signals are also available as outputs on the RTSI pins, as indicated in the *RTSI Triggers* section later in this chapter, and on the PFI pins, as indicated in [Chapter 4, Signal Connections](#).

Programmable Function Inputs

The 10 PFIs are connected to the signal routing multiplexer for each timing signal, and software can select one of the PFIs as the external source for a given timing signal. It is important to note that any of the PFIs can be used as an input by any of the timing signals and that multiple timing signals can use the same PFI simultaneously. This flexible routing scheme reduces the need to change physical connections to the I/O connector for different applications. You can also individually enable each of the PFI pins to output a specific internal timing signal. For example, if you need the UPDATE* signal as an output on the I/O connector, software can turn on the output driver for the PFI5/UPDATE* pin.

Board and RTSI Clocks

Many functions performed by the 611X E board require a frequency timebase to generate the necessary timing signals for controlling A/D conversions, DAC updates, or general-purpose signals at the I/O connector.

The 611X E board can use either its internal 20 MHz timebase or a timebase received over the RTSI bus. In addition, if you configure the board to use the internal timebase, you can also program the board to drive its internal timebase over the RTSI bus to another board that is programmed to receive this timebase signal. This clock source, whether local or from the RTSI bus, is used directly by the board as the primary frequency source. The default configuration at startup is to use the internal timebase without driving the RTSI bus timebase signal. This timebase is software selectable.

RTSI Triggers

The seven RTSI trigger lines on the RTSI bus provide a very flexible interconnection scheme for the 611X E board sharing the RTSI bus. These bidirectional lines can drive any of eight timing signals onto the RTSI bus and can receive any of these timing signals. This signal connection scheme is shown in Figure 3-12.

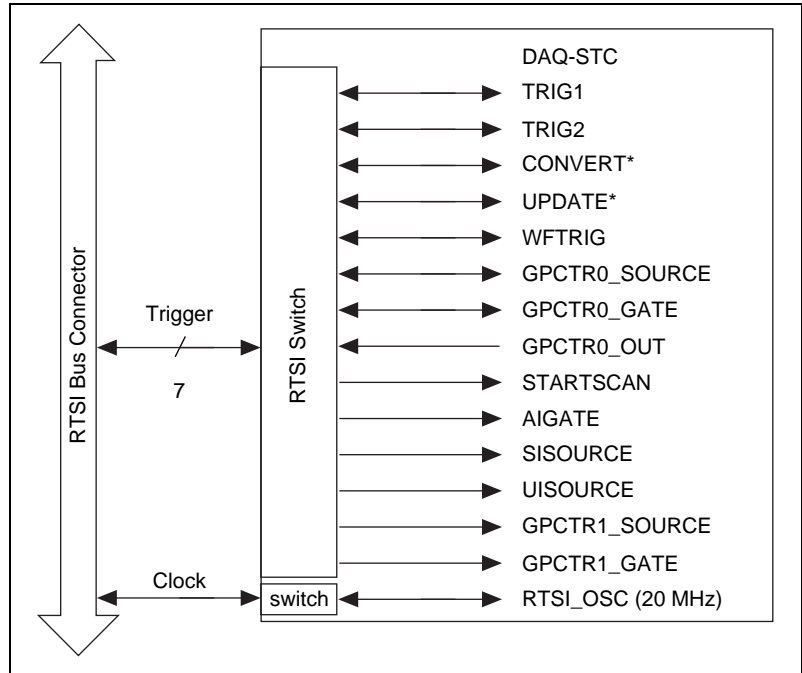


Figure 3-12. RTSI Bus Signal Connection

Refer to the *Timing Connections* section of [Chapter 4, Signal Connections](#), for a description of the signals shown in Figure 3-12.

Signal Connections

Chapter

4

This chapter describes how to make input and output signal connections to your 611X E board via the board I/O connector.

The I/O connector for the 611X E board has 68 pins that you can connect to 68-pin accessories with the SH6868EP shielded cable.

I/O Connector

Figure 4-1 shows the pin assignments for the 68-pin I/O connector on the 611X E board. A signal description follows the connector pinouts.



Caution: *Connections that exceed any of the maximum ratings of input or output signals on the 611X E board can damage the 611X E board and the computer. Maximum input ratings for each signal are given in the Protection column of Table 4-2. National Instruments is NOT liable for any damages resulting from such signal connections.*

ACH0-	34	68	ACH0+
ACH1+	33	67	ACH0GND
ACH1GND	32	66	ACH1-
ACH2- ¹	31	65	ACH2+ ¹
ACH3+ ¹	30	64	ACH2GND ¹
ACH3GND ¹	29	63	ACH3- ¹
NC	28	62	NC
NC	27	61	NC
NC	26	60	NC
NC	25	59	NC
NC	24	58	NC
NC	23	57	NC
DAC0OUT	22	56	NC
DAC1OUT	21	55	AOGND
NC	20	54	AOGND
DIO4	19	53	DGND
DGND	18	52	DIO0
DIO1	17	51	DIO5
DIO6	16	50	DGND
DGND	15	49	DIO2
+5 V	14	48	DIO7
DGND	13	47	DIO3
DGND	12	46	SCANCLK
PFI0/TRIG1	11	45	EXTSTROBE*
PFI1/TRIG2	10	44	DGND
DGND	9	43	PFI2/CONVERT*
+5 V	8	42	PFI3/GPCTR1_SOURCE
DGND	7	41	PFI4/GPCTR1_GATE
PFI5/UPDATE*	6	40	GPCTR1_OUT
PFI6/WFTRIG	5	39	DGND
DGND	4	38	PFI7/STARTSCAN
PFI9/GPCTR0_GATE	3	37	PFI8/GPCTR0_SOURCE
GPCTR0_OUT	2	36	DGND
FREQ_OUT	1	35	DGND

* 1 NC on PCI-6111E

Figure 4-1. I/O Connector Pin Assignment for the 611X E Board

I/O Connector Signal Descriptions

Table 4-1. Signal Descriptions for I/O Connector Pins

Signal Name	Reference	Direction	Description
ACH <0..3> GND	—	—	Analog Input Channels 0 through 3 ground—These pins are the bias current return point for differential measurements. ACH <2..3> GND signals are no connects on the PCI-6111E.
ACH<0..3> +	ACH <0..3> GND	Input	Analog Input Channels 0 through 3 (+)—These pins are routed to the (+) terminal of the respective channel's amplifier. ACH <2..3> + signals are no connects on the PCI-6111E.
ACH<0..3> –	ACH <0..3> GND	Input	Analog Input Channels 0 through 3 (–)—These pins are routed to the (–) terminal of the respective channel's amplifier. ACH <2..3> – signals are no connects on the PCI-6111E.
DAC0OUT	AOGND	Output	Analog Channel 0 Output—This pin supplies the voltage output of analog output channel 0.
DAC1OUT	AOGND	Output	Analog Channel 1 Output—This pin supplies the voltage output of analog output channel 1.
AOGND	—	—	Analog Output Ground—The analog output voltages are referenced to this node.
DGND	—	—	Digital Ground—This pin supplies the reference for the digital signals at the I/O connector as well as the +5 VDC supply.
DIO<0..7>	DGND	Input or Output	Digital I/O signals—DIO6 and 7 can control the up/down signal of general-purpose counters 0 and 1, respectively.
+5 V	DGND	Output	+5 VDC Source—These pins are fused for up to 1 A of +5 V supply. The fuse is self-resetting.
SCANCLK	DGND	Output	Scan Clock—This pin pulses once for each A/D conversion when enabled. The low-to-high edge indicates when the input signal can be removed from the input or switched to another signal.
EXTSTROBE*	DGND	Output	External Strobe—This output can be toggled under software control to latch signals or trigger events on external devices.

Table 4-1. Signal Descriptions for I/O Connector Pins (Continued)

Signal Name	Reference	Direction	Description
PFI0/TRIG1	DGND	Input	PFI0/Trigger 1—As an input, this is either one of the Programmable Function Inputs (PFIs) or the source for the hardware analog trigger. PFI signals are explained in the Timing Connections section later in this chapter. The hardware analog trigger is explained in the <i>Analog Trigger</i> section in Chapter 3, Hardware Overview .
		Output	As an output, this is the TRIG1 signal. In posttrigger data acquisition sequences, a low-to-high transition indicates the initiation of the acquisition sequence. In pretrigger applications, a low-to-high transition indicates the initiation of the pretrigger conversions.
PFI1/TRIG2	DGND	Input	PFI1/Trigger 2—As an input, this is one of the PFIs.
		Output	As an output, this is the TRIG2 signal. In pretrigger applications, a low-to-high transition indicates the initiation of the posttrigger conversions. TRIG2 is not used in posttrigger applications.
PFI2/CONVERT*	DGND	Input	PFI2/Convert—As an input, this is one of the PFIs.
		Output	As an output, this is the CONVERT* signal. A high-to-low edge on CONVERT* indicates that an A/D conversion is occurring.
PFI3/GPCTR1_SOURCE	DGND	Input	PFI3/Counter 1 Source—As an input, this is one of the PFIs.
		Output	As an output, this is the GPCTR1_SOURCE signal. This signal reflects the actual source connected to the general-purpose counter 1.
PFI4/GPCTR1_GATE	DGND	Input	PFI4/Counter 1 Gate—As an input, this is one of the PFIs.
		Output	As an output, this is the GPCTR1_GATE signal. This signal reflects the actual gate signal connected to the general-purpose counter 1.
GPCTR1_OUT	DGND	Output	Counter 1 Output—This output is from the general-purpose counter 1 output.
PFI5/UPDATE*	DGND	Input	PFI5/Update—As an input, this is one of the PFIs.
		Output	As an output, this is the UPDATE* signal. A high-to-low edge on UPDATE* indicates that the analog output primary group is being updated.

Table 4-1. Signal Descriptions for I/O Connector Pins (Continued)

Signal Name	Reference	Direction	Description
PFI6/WFTRIG	DGND	Input	PFI6/Waveform Trigger—As an input, this is one of the PFIs.
		Output	As an output, this is the WFTRIG signal. In timed analog output sequences, a low-to-high transition indicates the initiation of the waveform generation.
PFI7/STARTSCAN	DGND	Input	PFI7/Start of Scan—As an input, this is one of the PFIs.
		Output	As an output, this is the STARTSCAN signal. This pin pulses once at the start of each analog input scan in the interval scan. A low-to-high transition indicates the start of the scan.
PFI8/GPCTR0_SOURCE	DGND	Input	PFI8/Counter 0 Source—As an input, this is one of the PFIs.
		Output	As an output, this is the GPCTR0_SOURCE signal. This signal reflects the actual source connected to the general-purpose counter 0.
PFI9/GPCTR0_GATE	DGND	Input	PFI9/Counter 0 Gate—As an input, this is one of the PFIs.
		Output	As an output, this is the GPCTR0_GATE signal. This signal reflects the actual gate signal connected to the general-purpose counter 0.
GPCTR0_OUT	DGND	Output	Counter 0 Output—This output is from the general-purpose counter 0 output.
FREQ_OUT	DGND	Output	Frequency Output—This output is from the frequency generator output.

Table 4-2 shows the I/O signal summary for the 611X E boards.

Table 4-2. I/O Signal Summary for the 611X E

Signal Name	Signal Type and Direction	Impedance Input/ Output	Protection (Volts) On/Off	Source (mA at V)	Sink (mA at V)	Rise Time (ns)	Bias
ACH<0..3> +	AI	1 M Ω in parallel with 100 pF ¹ 1 M Ω in parallel with 10 pF ²	42 V	—	—	—	—
ACH<0..3> –	AI	10 nF	42 V	—	—	—	± 200 pA
ACH <0..3> GND	AI	—	—	—	—	—	—
DAC0OUT	AO	50 Ω	Short-circuit to ground	5 at 10	5 at -10	300 V/ μ s	—
DAC1OUT	AO	50 Ω	Short-circuit to ground	5 at 10	5 at -10	300 V/ μ s	—
AOGND	AO	—	—	—	—	—	—
DGND	DO	—	—	—	—	—	—
VCC	DO	0.1 Ω	Short-circuit to ground	1 A	—	—	—
DIO<0..7>	DIO	—	V _{cc} +0.5	13 at (V _{cc} -0.4)	24 at 0.4	1.1	50 k Ω pu
SCANCLK	DO	—	—	3.5 at (V _{cc} -0.4)	5 at 0.4	1.5	50 k Ω pu
EXTSTROBE*	DO	—	—	3.5 at (V _{cc} -0.4)	5 at 0.4	1.5	50 k Ω pu
PFI0/TRIG1	AI DIO	10 k Ω	± 35 V _{cc} +0.5	3.5 at (V _{cc} -0.4)	5 at 0.4	1.5	9 k Ω pu and 10 k Ω pd
PFI1/TRIG2	DIO	—	V _{cc} +0.5	3.5 at (V _{cc} -0.4)	5 at 0.4	1.5	50 k Ω pu
PFI2/CONVERT*	DIO	—	V _{cc} +0.5	3.5 at (V _{cc} -0.4)	5 at 0.4	1.5	50 k Ω pu
PFI3/GPCTR1_SOURCE	DIO	—	V _{cc} +0.5	3.5 at (V _{cc} -0.4)	5 at 0.4	1.5	50 k Ω pu

Table 4-2. I/O Signal Summary for the 611XE (Continued)

Signal Name	Signal Type and Direction	Impedance Input/Output	Protection (Volts) On/Off	Source (mA at V)	Sink (mA at V)	Rise Time (ns)	Bias
PFI4/GPCTR1_GATE	DIO	—	$V_{cc} + 0.5$	3.5 at ($V_{cc} - 0.4$)	5 at 0.4	1.5	50 k Ω pu
GPCTR1_OUT	DO	—	—	3.5 at ($V_{cc} - 0.4$)	5 at 0.4	1.5	50 k Ω pu
PFI5/UPDATE*	DIO	—	$V_{cc} + 0.5$	3.5 at ($V_{cc} - 0.4$)	5 at 0.4	1.5	50 k Ω pu
PFI6/WFTRIG	DIO	—	$V_{cc} + 0.5$	3.5 at ($V_{cc} - 0.4$)	5 at 0.4	1.5	50 k Ω pu
PFI7/STARTSCAN	DIO	—	$V_{cc} + 0.5$	3.5 at ($V_{cc} - 0.4$)	5 at 0.4	1.5	50 k Ω pu
PFI8/GPCTR0_SOURCE	DIO	—	$V_{cc} + 0.5$	3.5 at ($V_{cc} - 0.4$)	5 at 0.4	1.5	50 k Ω pu
PFI9/GPCTR0_GATE	DIO	—	$V_{cc} + 0.5$	3.5 at ($V_{cc} - 0.4$)	5 at 0.4	1.5	50 k Ω pu
GPCTR0_OUT	DO	—	—	3.5 at ($V_{cc} - 0.4$)	5 at 0.4	1.5	50 k Ω pu
FREQ_OUT	DO	—	—	3.5 at ($V_{cc} - 0.4$)	5 at 0.4	1.5	50 k Ω pu

¹ Applies to gain ≤ 1 , impedance refers to ACH<0..3>–
² Applies to gain > 1 , impedance refers to ACH<0..3>–
 AI = Analog Input, DIO = Digital Input/Output, pu = pull-up, AO = Analog Output, DO = Digital Output,
 AI/DIO = Analog Input/Digital Input/Output
 The tolerance on the 50 k Ω pull-up and pull-down resistors is very large. Actual value may range between 17 and 100 k Ω .

Analog Input Signal Connections

The analog input signals for the 611X E board are ACH<0..3>+ and ACH<0..3>-. The ACH<0..3>+ signals are routed to the positive input of the PGIA, and signals connected to ACH<0..3>- are routed to the negative input of the PGIA.



Caution: *Exceeding the differential and common-mode input ranges distorts your input signals. Exceeding the maximum input voltage rating can damage the 611X E board and the computer. National Instruments is NOT liable for any damages resulting from such signal connections. The maximum input voltage ratings are listed in the Protection column of Table 4-2.*

With the different configurations, you can use the PGIA in different ways. Figure 4-2 shows a diagram of your 611X E board PGIA.

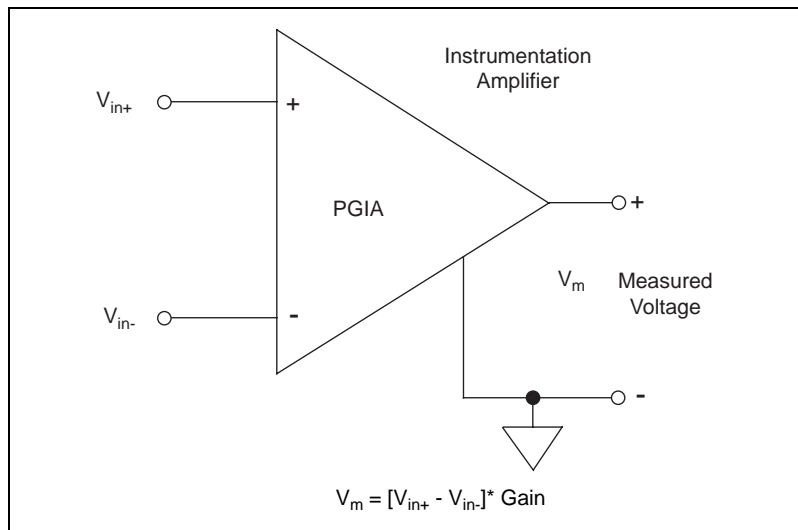


Figure 4-2. 611X E Board PGIA

The PGIA applies gain and common-mode voltage rejection and presents high input impedance to the analog input signals connected to the 611X E board. Signals are routed to the positive and negative inputs of the PGIA. The PGIA converts two input signals to a signal that is the difference between the two input signals multiplied by the gain setting of the amplifier. The amplifier output voltage is referenced to the ground for the board. The 611X E board A/D converter (ADC) measures this output voltage when it performs A/D conversions.

Types of Signal Sources

When making signal connections, you must first determine whether the signal sources are floating or ground-referenced. The following sections describe these two types of signals.

Floating Signal Sources

A floating signal source is not connected in any way to the building ground system but, rather, has an isolated ground-reference point. Some examples of floating signal sources are outputs of transformers, thermocouples, battery-powered devices, optical isolator outputs, and isolation amplifiers. An instrument or device that has an isolated output is a floating signal source. You must tie the ground reference of a floating signal to the 611X E board analog input ground to establish a local or onboard reference for the signal. Otherwise, the measured input signal varies as the source floats out of the common-mode input range.

Ground-Referenced Signal Sources

A ground-referenced signal source is connected in some way to the building system ground and is, therefore, already connected to a common ground point with respect to the 611X E board, assuming that the computer is plugged into the same power system. Nonisolated outputs of instruments and devices that plug into the building power system fall into this category.



The difference in ground potential between two instruments connected to the same building power system is typically between 1 and 100 mV but can be much higher if power distribution circuits are not properly connected. If a grounded signal source is improperly measured, this difference may appear as an error in the measurement. The connection instructions for grounded signal sources are designed to eliminate this ground potential difference from the measured signal.

Differential Measurements

The following sections discuss the use of differential (DIFF) measurements and considerations for measuring both floating and ground-referenced signal sources.

Table 4-3 summarizes the recommended DIFF signal connections and includes input examples for both types of signal sources.

Table 4-3. Signal Source Types

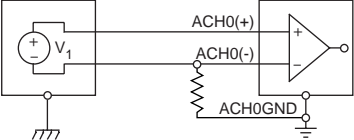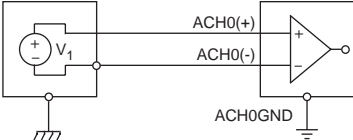DIFF Input Examples and Signal Source	Floating Signal Source (Not Connected to Building Ground)	Grounded Signal Source
Input Examples	<ul style="list-style-type: none"> • Ungrounded Thermocouples • Signal conditioning with isolated outputs • Battery devices 	<ul style="list-style-type: none"> • Plug-in cards with nonisolated outputs
Differential (DIFF)	 <p>See text for information on bias resistors.</p>	

Differential Connection Considerations

A differential connection is one in which the 611X E board analog input signal has its own reference signal or signal return path. The 611X E channels are always configured in DIFF input mode. The input signal is tied to the positive input of the PGIA, and its reference signal, or return, is tied to the negative input of the PGIA.

Each differential signal uses two inputs—one for the signal and one for its reference signal.

Differential signal connections reduce picked up noise and increase common-mode noise rejection. Differential signal connections also allow input signals to float within the common-mode limits of the PGIA.

Differential Connections for Ground-Referenced Signal Sources

Figure 4-3 shows how to connect a ground-referenced signal source to a channel on the 611X E board.

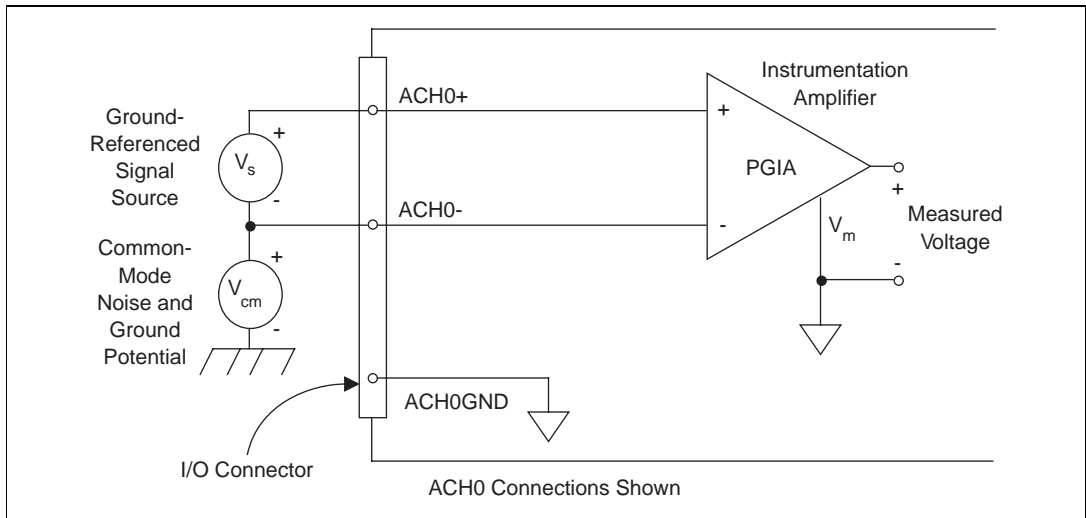


Figure 4-3. Differential Input Connections for Ground-Referenced Signals

With this type of connection, the PGIA rejects both the common-mode noise in the signal and the ground potential difference between the signal source and the 611X E board ground, shown as V_{cm} in Figure 4-3.

Differential Connections for Nonreferenced or Floating Signal Sources

Figure 4-4 shows how to connect a floating signal source to a channel on the 611X E board.

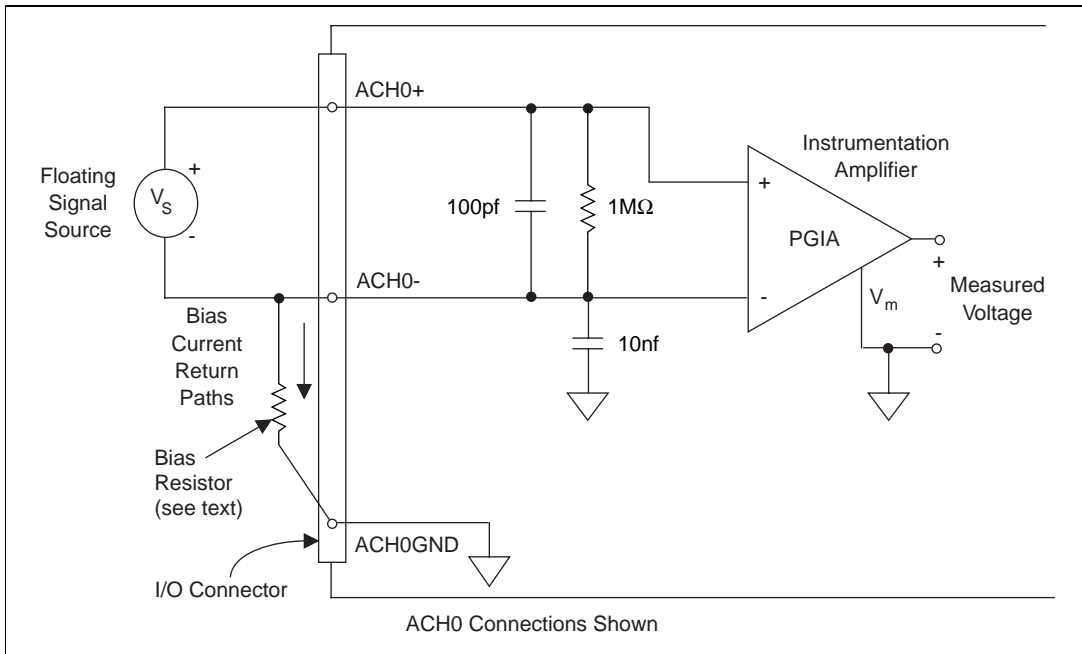


Figure 4-4. Differential Input Connections for Nonreferenced Signals

Figure 4-4 shows a bias resistor connected between $ACH0-$ and the floating signal source ground. If you do not use the resistor and the source is truly floating, the source is not likely to remain within the common-mode signal range of the PGIA, and the PGIA will saturate, causing erroneous readings. You must reference the source to the respective channel ground.

Common-Mode Signal Rejection Considerations

Figure 4-3 shows connections for signal sources that are already referenced to some ground point with respect to the 611X E board. In this case, the PGIA can reject any voltage caused by ground potential differences between the signal source and the board. In addition, with differential input connections, the PGIA can reject common-mode noise pickup in the leads connecting the signal sources to the board. The PGIA can reject common-mode signals as long as V_{in}^+ and V_{in}^- (input signals) are both within $\pm 11\text{ V}$ of the channel ground, for gain ≥ 1 . For gain < 1 , the input signals, for $ACH0+$, can be within $\pm 42\text{ V}$ of the channel ground.

Analog Output Signal Connections

The analog output signals are DAC0OUT, DAC1OUT, and AOGND.

DAC0OUT is the voltage output signal for analog output channel 0.

DAC1OUT is the voltage output signal for analog output channel 1.

AOGND is the ground reference signal for the analog output channels.

Figure 4-5 shows how to make analog output connections to the 611X E board.

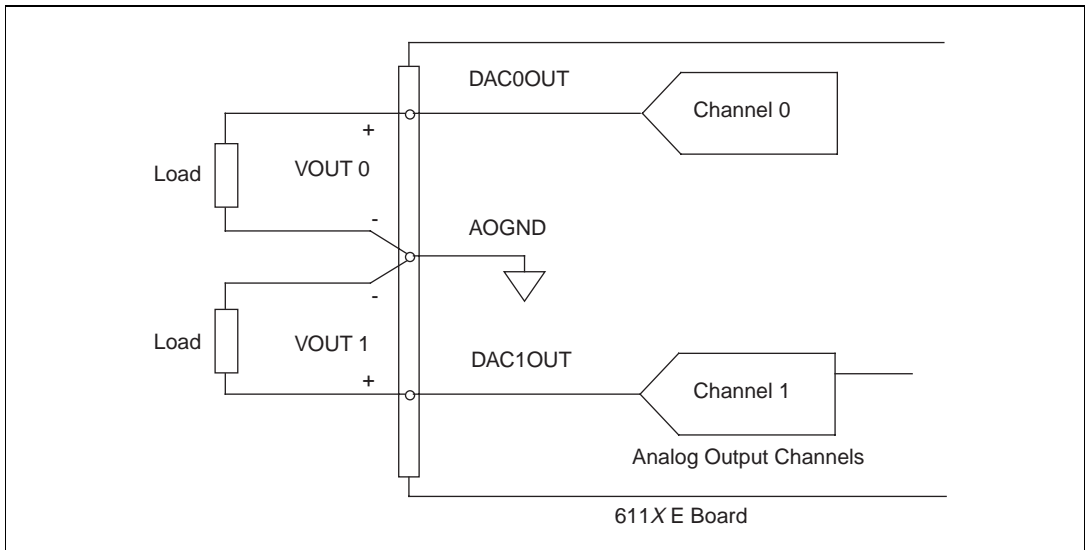


Figure 4-5. Analog Output Connections

Digital I/O Signal Connections

The digital I/O signals are DIO<0..7> and DGND. DIO<0..7> are the signals making up the DIO port, and DGND is the ground reference signal for the DIO port. You can program all lines individually to be inputs or outputs.



Caution: *Exceeding the maximum input voltage ratings, which are listed in Table 4-2, can damage the 611X E board and the computer. National Instruments is NOT liable for any damages resulting from such signal connections.*

Figure 4-6 shows signal connections for three typical digital I/O applications.

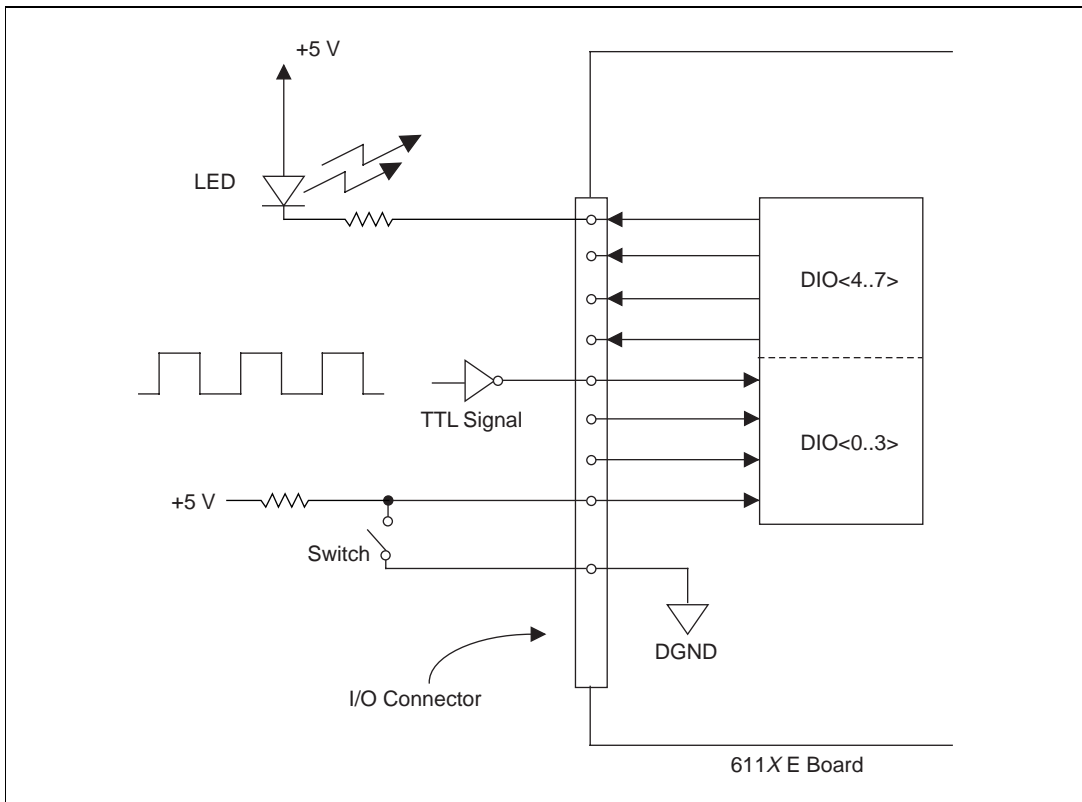


Figure 4-6. Digital I/O Connections

Figure 4-6 shows DIO<0..3> configured for digital input and DIO<4..7> configured for digital output. Digital input applications include receiving TTL signals and sensing external device states such as the switch state shown in Figure 4-6. Digital output applications include sending TTL signals and driving external devices such as the LED shown in Figure 4-6.

Power Connections

Two pins on the I/O connector supply +5 V from the computer power supply via a self-resetting fuse. The fuse will reset automatically within a few seconds after the overcurrent condition is removed. These pins are referenced to DGND and can be used to power external digital circuitry.

- Power rating +4.65 to +5.25 VDC at 1 A



Caution: *Under no circumstances should you connect these +5 V power pins directly to analog or digital ground or to any other voltage source on the 611X E board or any other device. Doing so can damage the 611X E board and the computer. National Instruments is NOT liable for damages resulting from such a connection.*

Timing Connections



Caution: *Exceeding the maximum input voltage ratings, which are listed in Table 4-2, can damage the 611X E board and the computer. National Instruments is NOT liable for any damages resulting from such signal connections.*

All external control over the timing of the 611X E board is routed through the 10 programmable function inputs labeled PFI0 through PFI9. These signals are explained in detail in the next section, [Programmable Function Input Connections](#). These PFIs are bidirectional; as outputs they are not programmable and reflect the state of many DAQ, waveform generation, and general-purpose timing signals. There are five other dedicated outputs for the remainder of the timing signals. As inputs, the PFI signals are programmable and can control any DAQ, waveform generation, and general-purpose timing signals.

The DAQ signals are explained in the [DAQ Timing Connections](#) section later in this chapter. The waveform generation signals are explained in the [Waveform Generation Timing Connections](#) section later in this chapter. The general-purpose timing signals are explained in the [General-Purpose Timing Signal Connections](#) section later in this chapter.

All digital timing connections are referenced to DGND. This reference is demonstrated in Figure 4-7, which shows how to connect an external TRIG1 source and an external CONVERT* source to two 611XE board PFI pins.

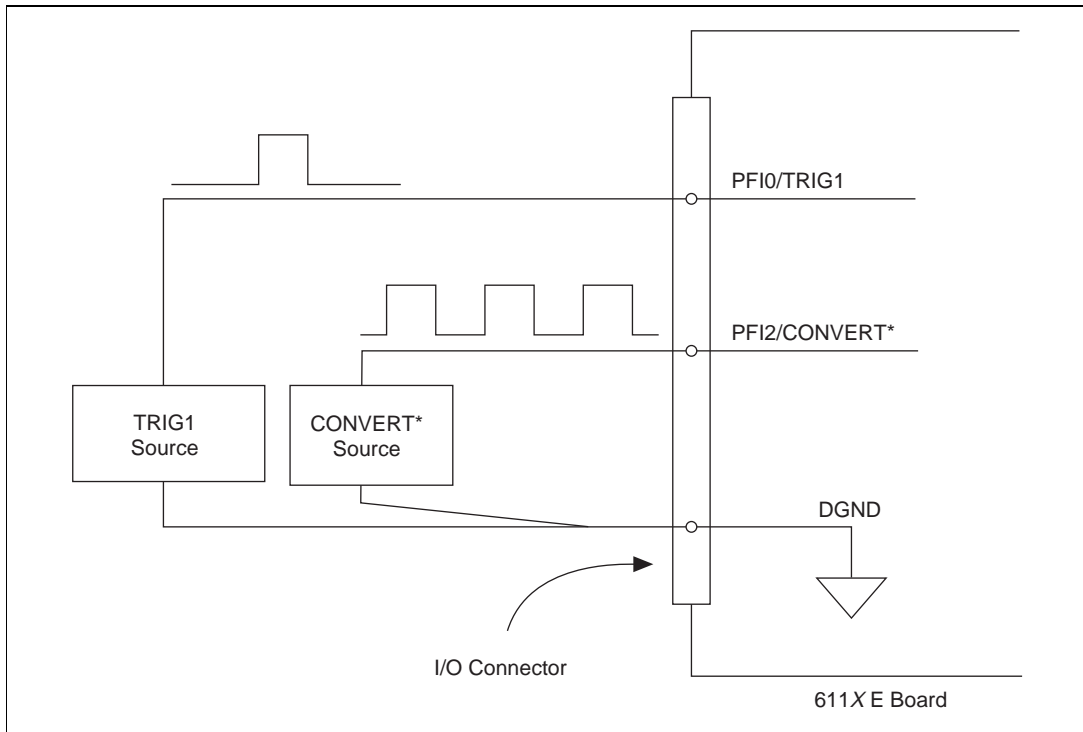


Figure 4-7. Timing I/O Connections

Programmable Function Input Connections

There are a total of 13 internal timing signals that you can externally control from the PFI pins. The source for each of these signals is software-selectable from any of the PFIs when you want external control. This flexible routing scheme reduces the need to change the physical wiring to the board I/O connector for different applications requiring alternative wiring.

You can individually enable each of the PFI pins to output a specific internal timing signal. For example, if you need the CONVERT* signal as an output on the I/O connector, software can turn on the output driver

for the PFI2/CONVERT* pin. Be careful not to drive a PFI signal externally when it is configured as an output.

As an input, you can individually configure each PFI for edge or level detection and for polarity selection, as well. You can use the polarity selection for any of the 13 timing signals, but the edge or level detection will depend upon the particular timing signal being controlled. The detection requirements for each timing signal are listed within the section that discusses that individual signal.

In edge-detection mode, the minimum pulse width required is 10 ns. This applies for both rising-edge and falling-edge polarity settings. There is no maximum pulse-width requirement in edge-detect mode.

In level-detection mode, there are no minimum or maximum pulse-width requirements imposed by the PFIs themselves, but there may be limits imposed by the particular timing signal being controlled. These requirements are listed later in this chapter.

DAQ Timing Connections

The DAQ timing signals are SCANCLK, EXTSTROBE*, TRIG1, TRIG2, STARTSCAN, CONVERT*, AIGATE, and SISOURCE.

Posttriggered data acquisition allows you to view only data that is acquired after a trigger event is received. A typical posttriggered DAQ sequence is shown in Figure 4-8. Pretriggered data acquisition allows you to view data that is acquired before the trigger of interest in addition to data acquired after the trigger. Figure 4-9 shows a typical pretriggered DAQ sequence. The description for each signal shown in these figures is included later in this chapter.

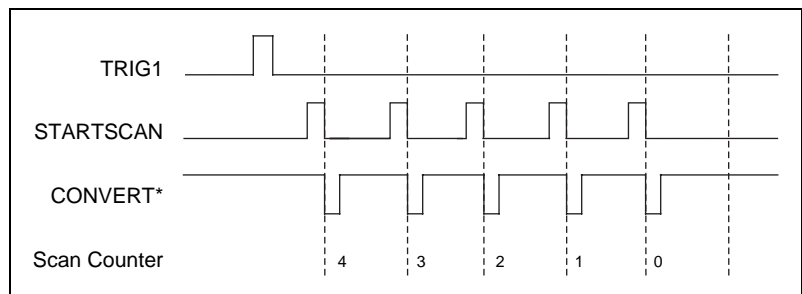


Figure 4-8. Typical Posttriggered Acquisition

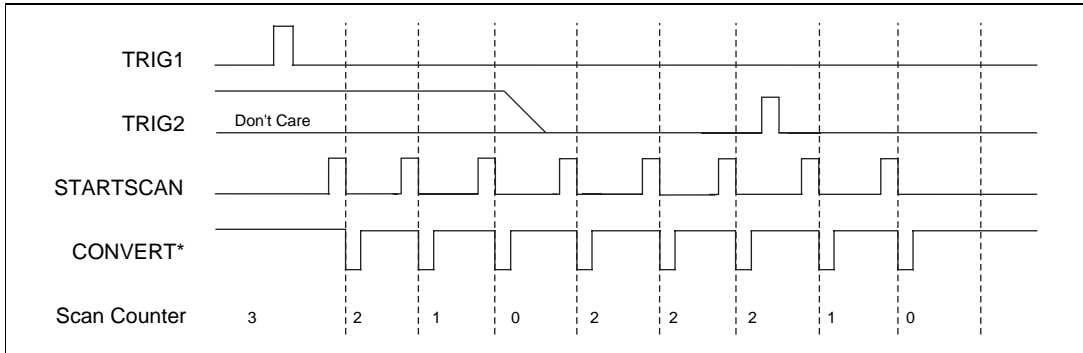


Figure 4-9. Typical Pretriggered Acquisition

SCANCLK Signal

SCANCLK is an output-only signal that generates a pulse with the leading edge occurring approximately 50 to 100 ns after an A/D conversion begins. The polarity of this output is software-selectable but is typically configured so that a low-to-high leading edge can clock external analog input multiplexers indicating when the input signal has been sampled and can be removed. This signal has a 450 ns pulse width and is software enabled. Figure 4-10 shows the timing for the SCANCLK signal.

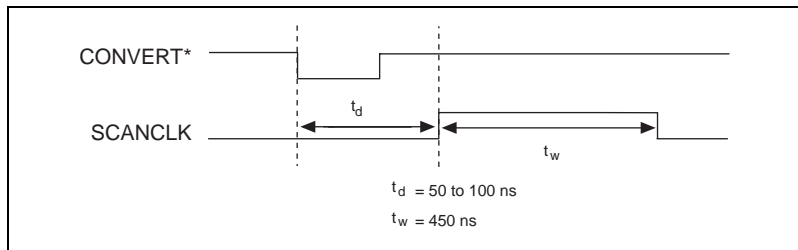


Figure 4-10. SCANCLK Signal Timing

EXTSTROBE* Signal

EXTSTROBE* is an output-only signal that generates either a single pulse or a sequence of eight pulses in the hardware-strobe mode. An external device can use this signal to latch signals or to trigger events. In the single-pulse mode, software controls the level of the EXTSTROBE* signal. A 10 μ s and a 1.2 μ s clock are available for generating a sequence of eight pulses in the hardware-strobe mode.

Figure 4-11 shows the timing for the hardware-strobe mode EXTSTROBE* signal.

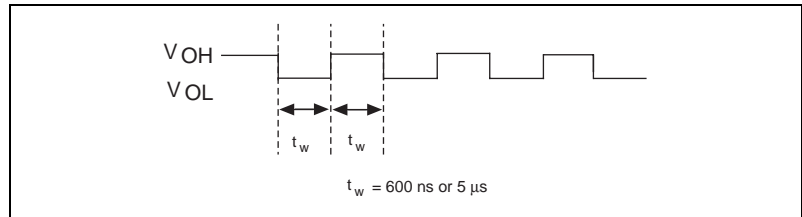


Figure 4-11. EXTSTROBE* Signal Timing

TRIG1 Signal

Any PFI pin can externally input the TRIG1 signal, which is available as an output on the PFI0/TRIG1 pin.

Refer to Figures 4-8 and 4-9 for the relationship of TRIG1 to the DAQ sequence.

As an input, the TRIG1 signal is configured in the edge-detection mode. You can select any PFI pin as the source for TRIG1 and configure the polarity selection for either rising or falling edge. The selected edge of the TRIG1 signal starts the data acquisition sequence for both posttriggered and pretriggered acquisitions. The 611X E supports analog triggering on the PFI0/TRIG1 pin. See [Chapter 3, Hardware Overview](#), for more information on analog triggering.

As an output, the TRIG1 signal reflects the action that initiates a DAQ sequence. This is true even if the acquisition is being externally triggered by another PFI. The output is an active high pulse with a pulse width of 25 to 50 ns. This output is set to tri-state at startup.

Figures 4-12 and 4-13 show the input and output timing requirements for the TRIG1 signal.

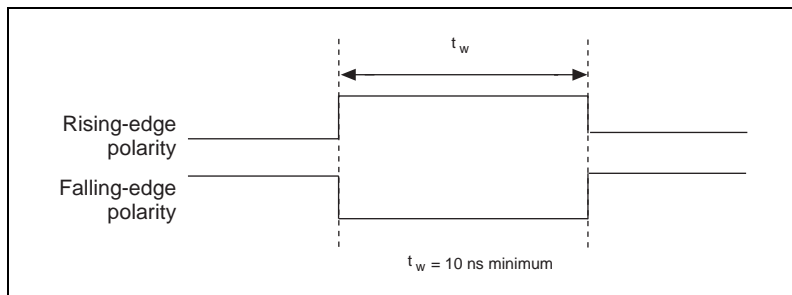


Figure 4-12. TRIG1 Input Signal Timing

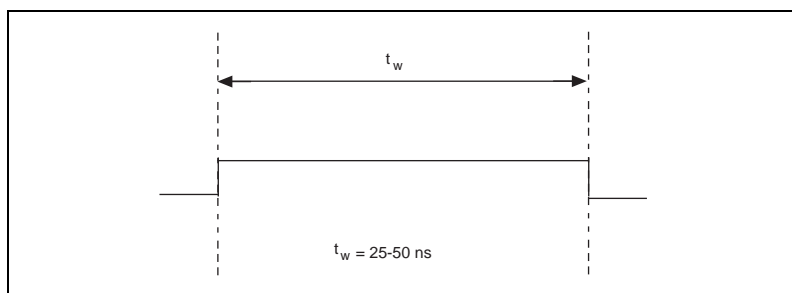


Figure 4-13. TRIG1 Output Signal Timing

The board also uses the TRIG1 signal to initiate pretriggered DAQ operations. In most pretriggered applications, the TRIG1 signal is generated by a software trigger. Refer to the TRIG2 signal description for a complete description of the use of TRIG1 and TRIG2 in a pretriggered DAQ operation.

TRIG2 Signal

Any PFI pin can externally input the TRIG2 signal, which is available as an output on the PFI1/TRIG2 pin. Refer to Figure 4-9 for the relationship of TRIG2 to the DAQ sequence.

As an input, the TRIG2 signal is configured in the edge-detection mode. You can select any PFI pin as the source for TRIG2 and configure the polarity selection for either rising or falling edge. The selected edge of the TRIG2 signal initiates the posttriggered phase of a pretriggered acquisition sequence. In pretriggered mode, the TRIG1 signal initiates the data acquisition. The scan counter indicates the minimum number

of scans before TRIG2 can be recognized. After the scan counter decrements to zero, it is loaded with the number of posttrigger scans to acquire while the acquisition continues. The board ignores the TRIG2 signal if it is asserted prior to the scan counter decrementing to zero. After the selected edge of TRIG2 is received, the board will acquire a fixed number of scans and the acquisition will stop. This mode acquires data both before and after receiving TRIG2.

As an output, the TRIG2 signal reflects the posttrigger in a pretriggered acquisition sequence. This is true even if the acquisition is being externally triggered by another PFI. The TRIG2 signal is not used in posttriggered data acquisition. The output is an active high pulse with a pulse width of 25 to 50 ns. This output is set to tri-state at startup.

Figures 4-14 and 4-15 show the input and output timing requirements for the TRIG2 signal.

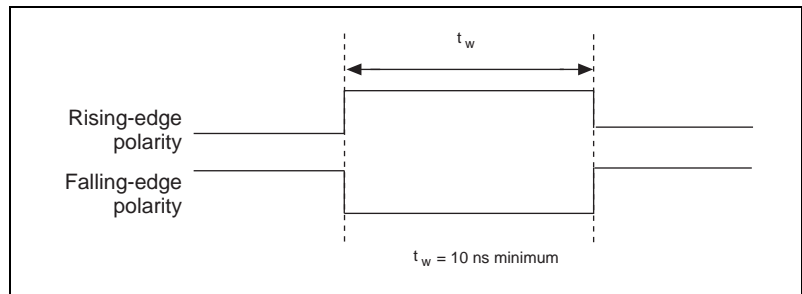


Figure 4-14. TRIG2 Input Signal Timing

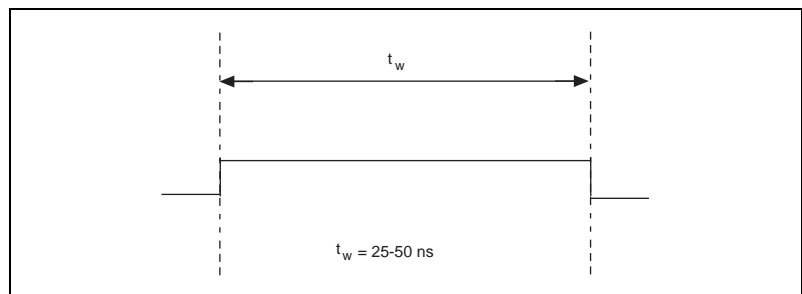


Figure 4-15. TRIG2 Output Signal Timing

STARTSCAN Signal

Any PFI pin can externally input the STARTSCAN signal, which is available as an output on the PFI7/STARTSCAN pin. Refer to Figures 4-8 and 4-9 for the relationship of STARTSCAN to the DAQ sequence.

As an input, the STARTSCAN signal is configured in the edge-detection mode. You can select any PFI pin as the source for STARTSCAN and configure the polarity selection for either rising or falling edge. The selected edge of the STARTSCAN signal initiates a scan. The sample interval counter starts if you select internally triggered CONVERT*.

As an output, the STARTSCAN signal reflects the actual start pulse that initiates a scan. This is true even if the starts are being externally triggered by another PFI. You have two output options. The first is an active high pulse with a pulse width of 25 to 50 ns, which indicates the start of the scan. The second action is an active high pulse that terminates at the start of the last conversion in the scan, which indicates a scan in progress. STARTSCAN will be deasserted t_{off} after the last conversion in the scan is initiated. This output is set to tri-state at startup.

Figures 4-16 and 4-17 show the input and output timing requirements for the STARTSCAN signal.

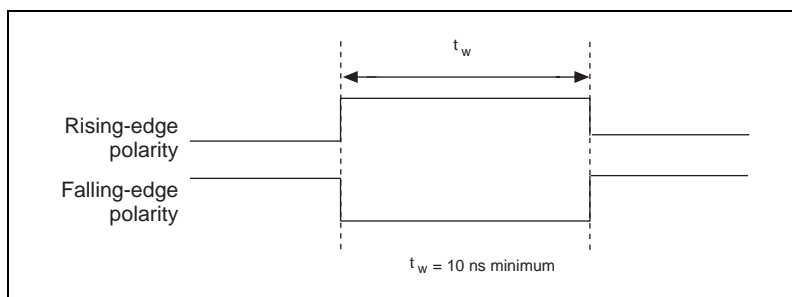


Figure 4-16. STARTSCAN Input Signal Timing

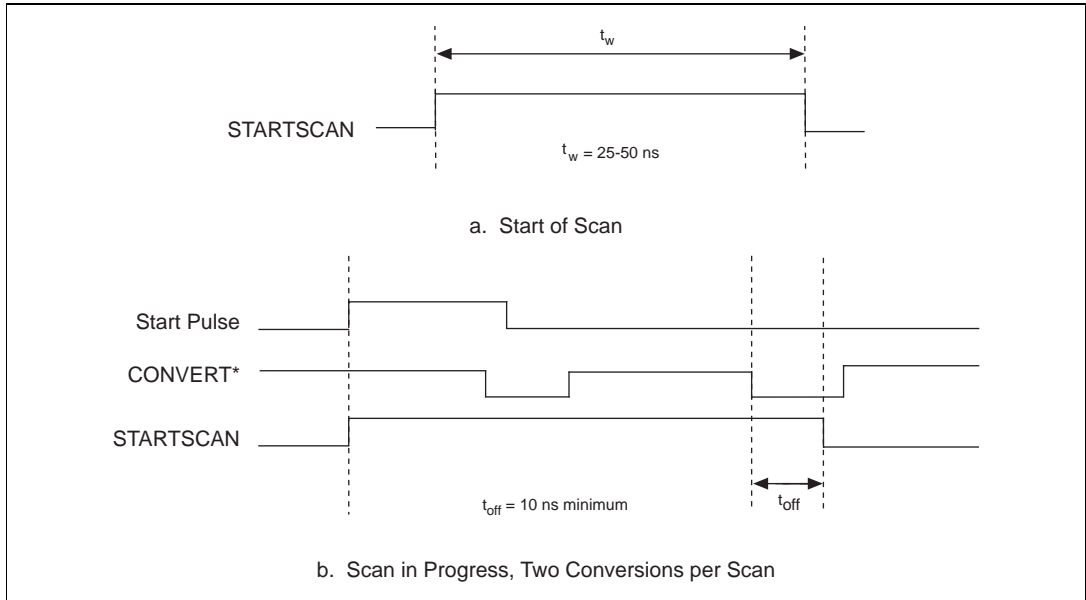


Figure 4-17. STARTSCAN Output Signal Timing

The CONVERT* pulses are masked off until the board generates the STARTSCAN signal. If you are using internally generated conversions, the first CONVERT* appears when the onboard sample interval counter reaches zero. If you select an external CONVERT*, the first external pulse after STARTSCAN generates a conversion. The STARTSCAN pulses should be separated by at least one scan period.

A counter on the 611X E board internally generates the STARTSCAN signal unless you select some external source. This counter is started by the TRIG1 signal and is stopped either by software or by the sample counter.

Scans generated by either an internal or external STARTSCAN signal are inhibited unless they occur within a DAQ sequence. Scans occurring within a DAQ sequence may be gated by either the hardware (AIGATE) signal or software command register gate.

CONVERT* Signal

Any PFI pin can externally input the CONVERT* signal, which is available as an output on the PFI2/CONVERT* pin.

Refer to Figures 4-8 and 4-9 for the relationship of STARTSCAN to the DAQ sequence.

As an input, the CONVERT* signal is configured in the edge-detection mode. You can select any PFI pin as the source for CONVERT* and configure the polarity selection for either rising or falling edge. The selected edge of the CONVERT* signal initiates an A/D conversion.

As an output, the CONVERT* signal reflects the actual convert pulse that is connected to the ADC. This is true even if the conversions are being externally generated by another PFI. The output is an active low pulse with a pulse width of 50 to 100 ns. This output is set to tri-state at startup.

Figures 4-18 and 4-19 show the input and output timing requirements for the CONVERT* signal.

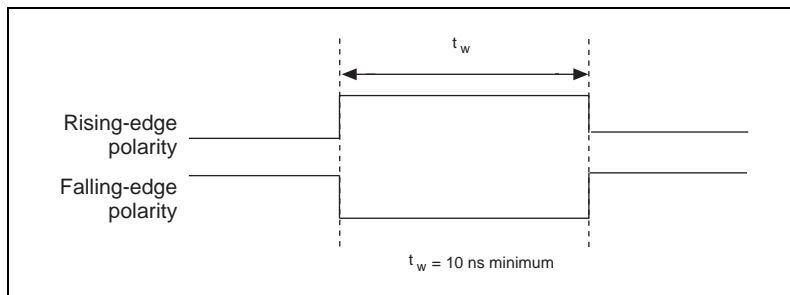


Figure 4-18. CONVERT* Input Signal Timing

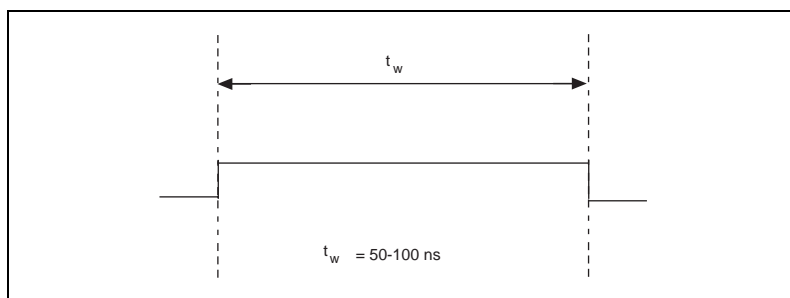


Figure 4-19. CONVERT* Output Signal Timing

The ADC switches to hold mode within 20 ns of the selected edge. This hold-mode delay time is a function of temperature and does not vary from one conversion to the next.

The sample interval counter on the 611XE board normally generates the CONVERT* signal unless you select some external source. The counter is started by the STARTSCAN signal and continues to count down and reload itself until the scan is finished. It then reloads itself in preparation for the next STARTSCAN pulse.

A/D conversions generated by either an internal or external CONVERT* signal are inhibited unless they occur within a DAQ sequence. Scans occurring within a DAQ sequence may be gated by either the hardware (AIGATE) signal or software command register gate.

AIGATE Signal

Any PFI pin can externally input the AIGATE signal, which is not available as an output on the I/O connector. The AIGATE signal can mask off scans in a DAQ sequence. You can configure the PFI pin you select as the source for the AIGATE signal in either the level-detection or edge-detection mode. You can configure the polarity selection for the PFI pin for either active high or active low.

In the level-detection mode if AIGATE is active, the STARTSCAN signal is masked off and no scans can occur. In the edge-detection mode, the first active edge disables the STARTSCAN signal, and the second active edge enables STARTSCAN.

The AIGATE signal can neither stop a scan in progress nor continue a previously gated-off scan; in other words, once a scan has started, AIGATE does not gate off conversions until the beginning of the next scan and, conversely, if conversions are being gated off, AIGATE does not gate them back on until the beginning of the next scan.

SISOURCE Signal

Any PFI pin can externally input the SISOURCE signal, which is not available as an output on the I/O connector. The onboard scan interval counter uses the SISOURCE signal as a clock to time the generation of the STARTSCAN signal. You must configure the PFI pin you select as the source for the SISOURCE signal in the level-detection mode. You can configure the polarity selection for the PFI pin for either active high or active low.

The maximum allowed frequency is 20 MHz, with a minimum pulse width of 23 ns high or low. There is no minimum frequency limitation.

Either the 20 MHz or 100 kHz internal timebase generates the SISOURCE signal unless you select some external source. Figure 4-20 shows the timing requirements for the SISOURCE signal.

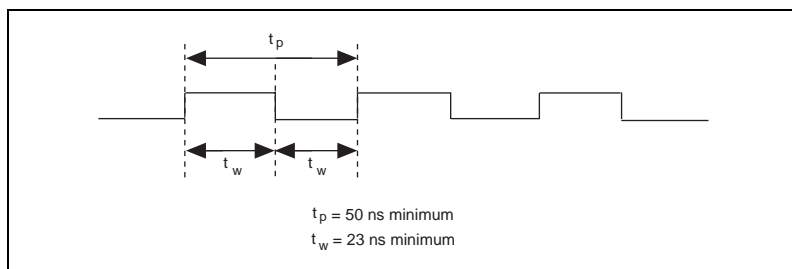


Figure 4-20. SISOURCE Signal Timing

Waveform Generation Timing Connections

The analog group defined for the 611X E board is controlled by WFTRIG, UPDATE*, and UISOURCE.

WFTRIG Signal

Any PFI pin can externally input the WFTRIG signal, which is available as an output on the PFI6/WFTRIG pin.

As an input, the WFTRIG signal is configured in the edge-detection mode. You can select any PFI pin as the source for WFTRIG and configure the polarity selection for either rising or falling edge. The selected edge of the WFTRIG signal starts the waveform generation for the DACs. The update interval (UI) counter is started if you select internally generated UPDATE*.

As an output, the WFTRIG signal reflects the trigger that initiates waveform generation. This is true even if the waveform generation is being externally triggered by another PFI. The output is an active high pulse with a pulse width of 25 to 50 ns. This output is set to tri-state at startup.

Figures 4-21 and 4-22 show the input and output timing requirements for the WFTRIG signal.

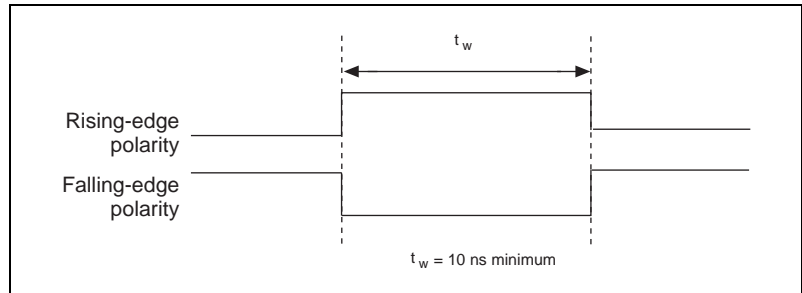


Figure 4-21. WFTRIG Input Signal Timing

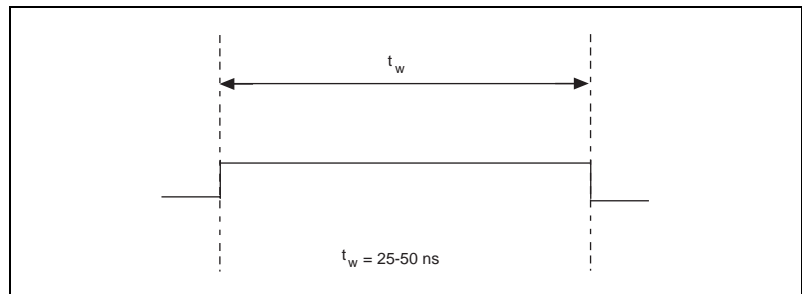


Figure 4-22. WFTRIG Output Signal Timing

UPDATE* Signal

Any PFI pin can externally input the UPDATE* signal, which is available as an output on the PFI5/UPDATE* pin.

As an input, the UPDATE* signal is configured in the edge-detection mode. You can select any PFI pin as the source for UPDATE* and configure the polarity selection for either rising or falling edge. The selected edge of the UPDATE* signal updates the outputs of the DACs. In order to use UPDATE*, you must set the DACs to posted-update mode.

As an output, the UPDATE* signal reflects the actual update pulse that is connected to the DACs. This is true even if the updates are being externally generated by another PFI. The output is an active low pulse with a pulse width of 50 to 75 ns. This output is set to tri-state at startup.

Figures 4-23 and 4-24 show the input and output timing requirements for the UPDATE* signal.

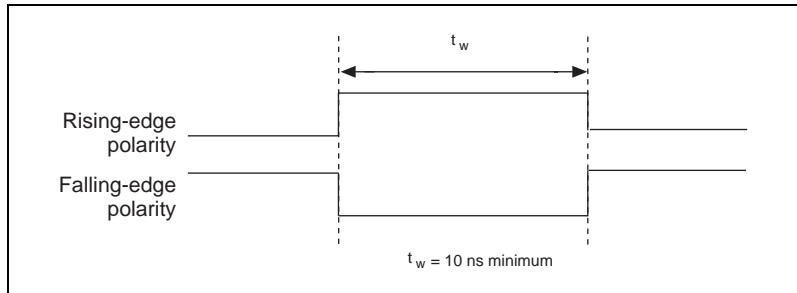


Figure 4-23. UPDATE* Input Signal Timing

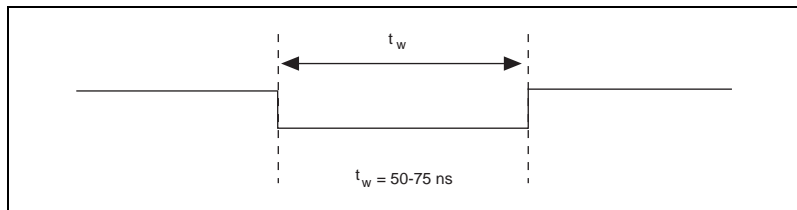


Figure 4-24. UPDATE* Output Signal Timing

The DACs are updated within 100 ns of the leading edge. Separate the UPDATE* pulses with enough time that new data can be written to the DAC latches.

The UI counter for the 611XE board normally generates the UPDATE* signal unless you select some external source. The UI counter is started by the WFTRIG signal and can be stopped by software or the internal Buffer Counter.

D/A conversions generated by either an internal or external UPDATE* signal do not occur when gated by the software command register gate.

UISOURCE Signal

Any PFI pin can externally input the UISOURCE signal, which is not available as an output on the I/O connector. The UI counter uses the UISOURCE signal as a clock to time the generation of the UPDATE* signal. You must configure the PFI pin you select as the source for the UISOURCE signal in the level-detection mode. You can configure the

polarity selection for the PFI pin for either active high or active low. Figure 4-25 shows the timing requirements for the UISOURCE signal.

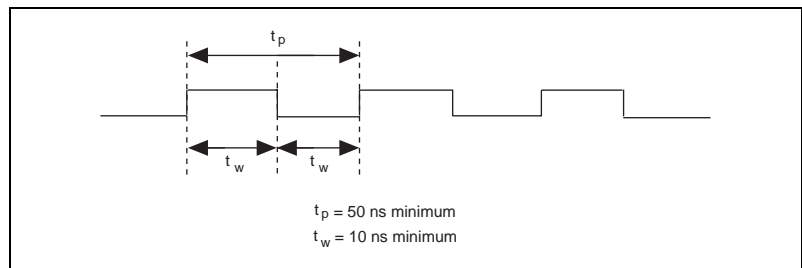


Figure 4-25. UISOURCE Signal Timing

The maximum allowed frequency is 20 MHz, with a minimum pulse width of 10 ns high or low. There is no minimum frequency limitation.

Either the 20 MHz or 100 kHz internal timebase normally generates the UISOURCE signal unless you select some external source.

General-Purpose Timing Signal Connections

The general-purpose timing signals are GPCTR0_SOURCE, GPCTR0_GATE, GPCTR0_OUT, GPCTR0_UP_DOWN, GPCTR1_SOURCE, GPCTR1_GATE, GPCTR1_OUT, GPCTR1_UP_DOWN, and FREQ_OUT.

GPCTR0_SOURCE Signal

Any PFI pin can externally input the GPCTR0_SOURCE signal, which is available as an output on the PFI8/GPCTR0_SOURCE pin.

As an input, the GPCTR0_SOURCE signal is configured in the edge-detection mode. You can select any PFI pin as the source for GPCTR0_SOURCE and configure the polarity selection for either rising or falling edge.

As an output, the GPCTR0_SOURCE signal reflects the actual clock connected to general-purpose counter 0. This is true even if another PFI is externally inputting the source clock. This output is set to tri-state at startup.

Figure 4-26 shows the timing requirements for the GPCTR0_SOURCE signal.

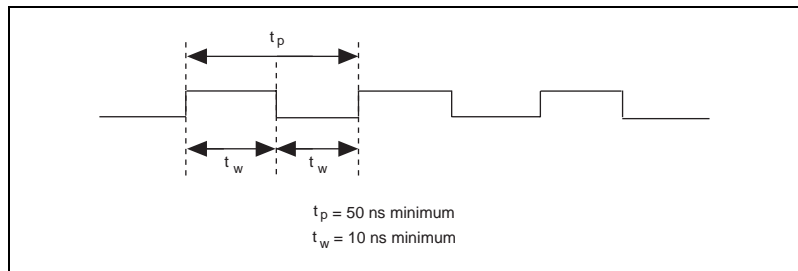


Figure 4-26. GPCTR0_SOURCE Signal Timing

The maximum allowed frequency is 20 MHz, with a minimum pulse width of 10 ns high or low. There is no minimum frequency limitation.

The 20 MHz or 100 kHz timebase normally generates the GPCTR0_SOURCE signal unless you select some external source.

GPCTR0_GATE Signal

Any PFI pin can externally input the GPCTR0_GATE signal, which is available as an output on the PFI9/GPCTR0_GATE pin.

As an input, the GPCTR0_GATE signal is configured in the edge-detection mode. You can select any PFI pin as the source for GPCTR0_GATE and configure the polarity selection for either rising or falling edge. You can use the gate signal in a variety of different applications to perform actions such as starting and stopping the counter, generating interrupts, saving the counter contents, and so on.

As an output, the GPCTR0_GATE signal reflects the actual gate signal connected to general-purpose counter 0. This is true even if the gate is being externally generated by another PFI. This output is set to tri-state at startup.

Figure 4-27 shows the timing requirements for the GPCTR0_GATE signal.

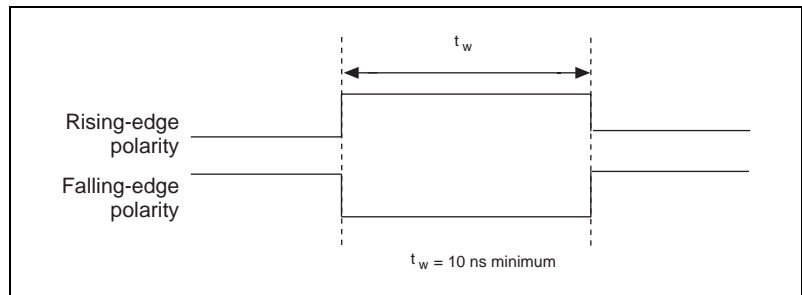


Figure 4-27. GPCTR0_GATE Signal Timing in Edge-Detection Mode

GPCTR0_OUT Signal

This signal is available only as an output on the GPCTR0_OUT pin. The GPCTR0_OUT signal reflects the terminal count (TC) of general-purpose counter 0. You have two software-selectable output options—pulse on TC and toggle output polarity on TC. The output polarity is software selectable for both options. This output is set to tri-state at startup. Figure 4-28 shows the timing of the GPCTR0_OUT signal.

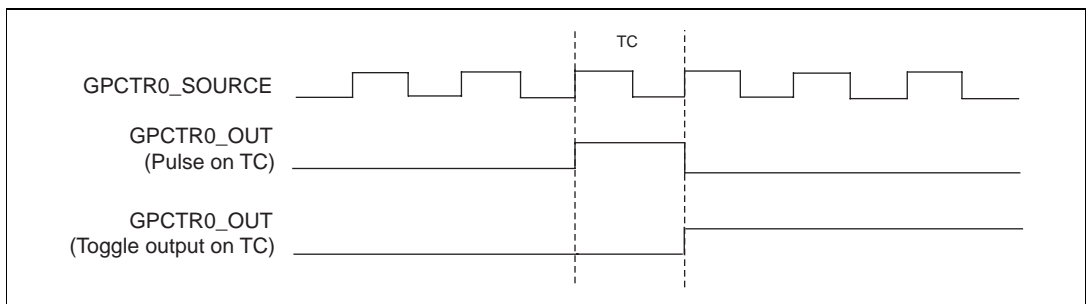


Figure 4-28. GPCTR0_OUT Signal Timing

GPCTR0_UP_DOWN Signal

This signal can be externally input on the DIO6 pin and is not available as an output on the I/O connector. The general-purpose counter 0 will count down when this pin is at a logic low and count up when it is at a logic high. You can disable this input so that software can control the up-down functionality and leave the DIO6 pin free for general use.

GPCTR1_SOURCE Signal

Any PFI pin can externally input the GPCTR1_SOURCE signal, which is available as an output on the PFI3/GPCTR1_SOURCE pin.

As an input, the GPCTR1_SOURCE signal is configured in the edge-detection mode. You can select any PFI pin as the source for GPCTR1_SOURCE and configure the polarity selection for either rising or falling edge.

As an output, the GPCTR1_SOURCE monitors the actual clock connected to general-purpose counter 1. This is true even if the source clock is being externally generated by another PFI. This output is set to tri-state at startup.

Figure 4-29 shows the timing requirements for the GPCTR1_SOURCE signal.

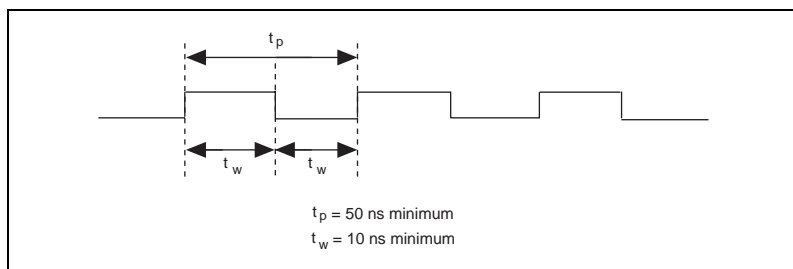


Figure 4-29. GPCTR1_SOURCE Signal Timing

The maximum allowed frequency is 20 MHz, with a minimum pulse width of 10 ns high or low. There is no minimum frequency limitation.

The 20 MHz or 100 kHz timebase normally generates the GPCTR1_SOURCE unless you select some external source.

GPCTR1_GATE Signal

Any PFI pin can externally input the GPCTR1_GATE signal, which is available as an output on the PFI4/GPCTR1_GATE pin.

As an input, the GPCTR1_GATE signal is configured in edge-detection mode. You can select any PFI pin as the source for GPCTR1_GATE and configure the polarity selection for either rising or falling edge. You can use the gate signal in a variety of different applications to perform such

actions as starting and stopping the counter, generating interrupts, saving the counter contents, and so on.

As an output, the GPCTR1_GATE signal monitors the actual gate signal connected to general-purpose counter 1. This is true even if the gate is being externally generated by another PFI. This output is set to tri-state at startup.

Figure 4-30 shows the timing requirements for the GPCTR1_GATE signal.

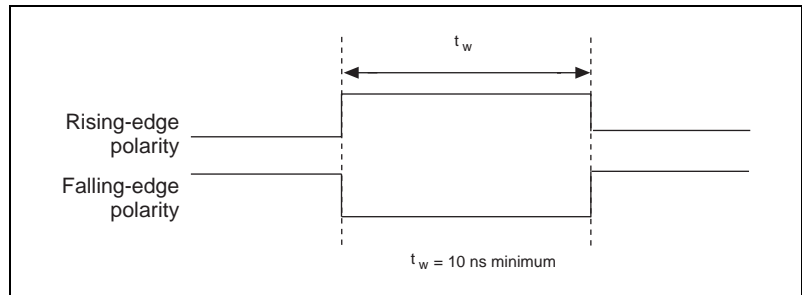


Figure 4-30. GPCTR1_GATE Signal Timing in Edge-Detection Mode

GPCTR1_OUT Signal

This signal is available only as an output on the GPCTR1_OUT pin. The GPCTR1_OUT signal monitors the TC board general-purpose counter 1. You have two software-selectable output options—pulse on TC and toggle output polarity on TC. The output polarity is software selectable for both options. This output is set to tri-state at startup. Figure 4-31 shows the timing requirements for the GPCTR1_OUT signal.

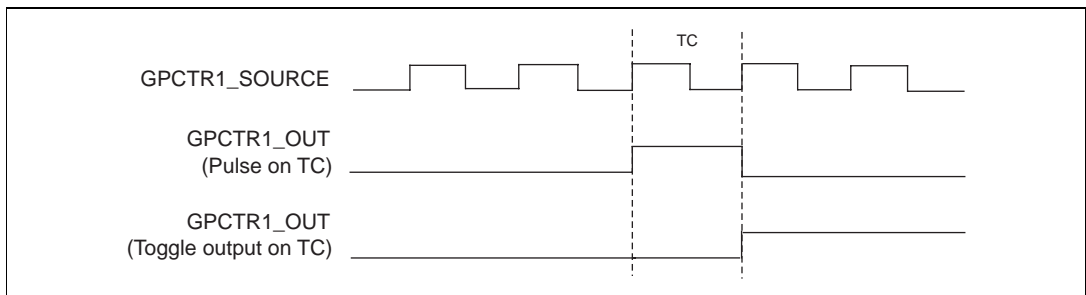


Figure 4-31. GPCTR1_OUT Signal Timing

GPCTR1_UP_DOWN Signal

This signal can be externally input on the DIO7 pin and is not available as an output on the I/O connector. General-purpose counter 1 counts down when this pin is at a logic low and counts up at a logic high. This input can be disabled so that software can control the up-down functionality and leave the DIO7 pin free for general use. Figure 4-32 shows the timing requirements for the GATE and SOURCE input signals and the timing specifications for the 611X E board OUT output signals.

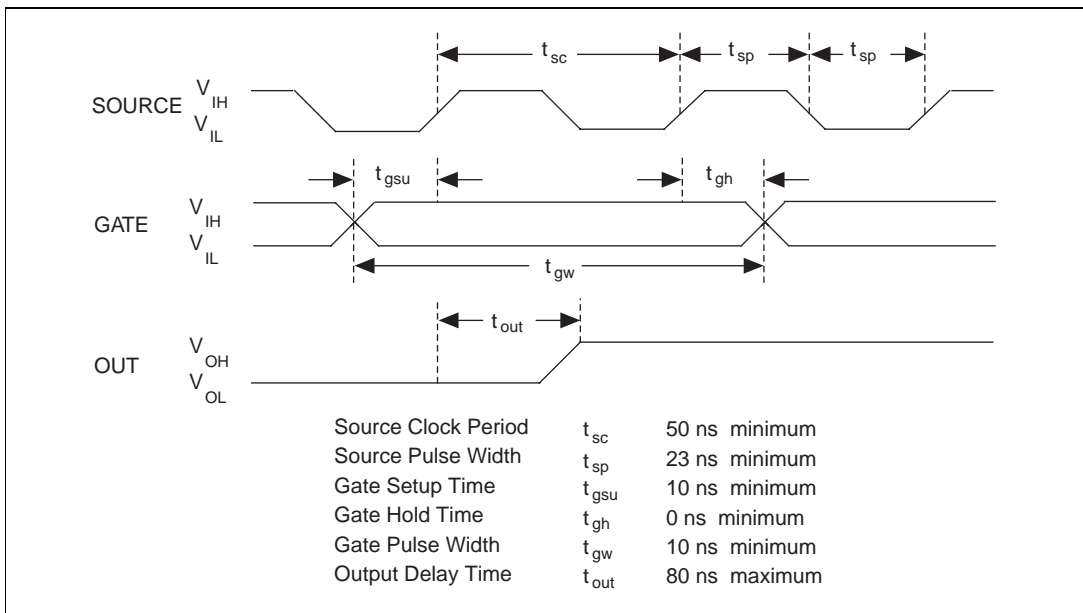


Figure 4-32. GPCTR Timing Summary

The GATE and OUT signal transitions shown in Figure 4-32 are referenced to the rising edge of the SOURCE signal. This timing diagram assumes that the counters are programmed to count rising edges. The same timing diagram, but with the source signal inverted and referenced to the falling edge of the source signal, would apply when the counter is programmed to count falling edges.

The GATE input timing parameters are referenced to the signal at the SOURCE input or to one of the internally generated signals on the 611X E board. Figure 4-32 shows the GATE signal referenced to the rising edge of a source signal. The gate must be valid (either high or

low) for at least 10 ns before the rising or falling edge of a source signal for the gate to take effect at that source edge, as shown by t_{gsu} and t_{gh} in Figure 4-32. The gate signal is not required to be held after the active edge of the source signal.

If you use an internal timebase clock, the gate signal cannot be synchronized with the clock. In this case, gates applied close to a source edge take effect either on that source edge or on the next one. This arrangement results in an uncertainty of one source clock period with respect to unsynchronized gating sources.

The OUT output timing parameters are referenced to the signal at the SOURCE input or to one of the internally generated clock signals on the 611X E board. Figure 4-32 shows the OUT signal referenced to the rising edge of a source signal. Any OUT signal state changes occur within 80 ns after the rising or falling edge of the source signal.

FREQ_OUT Signal

This signal is available only as an output on the FREQ_OUT pin. The frequency generator for the 611X E board outputs the FREQ_OUT pin. The frequency generator is a 4-bit counter that can divide its input clock by the numbers 1 through 16. The input clock of the frequency generator is software-selectable from the internal 10 MHz and 100 kHz timebases. The output polarity is software selectable. This output is set to tri-state at startup.

Field Wiring Considerations

Environmental noise can seriously affect the accuracy of measurements made with the 611X E board if you do not take proper care when running signal wires between signal sources and the board. The following recommendations apply mainly to analog input signal routing to the board, although they also apply to signal routing in general.

Minimize noise pickup and maximize measurement accuracy by taking the following precautions:

- Use differential analog input connections to reject common-mode noise.
- Use individually shielded, twisted-pair wires to connect analog input signals to the board. With this type of wire, the signals attached to the ACH+ and ACH- inputs are twisted together and then covered with a shield. You then connect this shield only at one

point to the signal source ground. This kind of connection is required for signals traveling through areas with large magnetic fields or high electromagnetic interference.

- Route signals to the board carefully. Keep cabling away from noise sources. The most common noise source in a PCI data acquisition system is the video monitor. Separate the monitor from the analog signals as much as possible.

The following recommendations apply for all signal connections to the 611X E board:

- Separate the 611X E board signal lines from high-current or high-voltage lines. These lines can induce currents in or voltages on the 611X E board signal lines if they run in parallel paths at a close distance. To reduce the magnetic coupling between lines, separate them by a reasonable distance if they run in parallel, or run the lines at right angles to each other.
- Do not run signal lines through conduits that also contain power lines.
- Protect signal lines from magnetic fields caused by electric motors, welding equipment, breakers, or transformers by running them through special metal conduits.

For more information, refer to the application note, *Field Wiring and Noise Consideration for Analog Signals*, available from National Instruments.

Calibration

Chapter

5

This chapter discusses the calibration procedures for your 611X E board. If you are using the NI-DAQ device driver, that software includes calibration functions for performing all of the steps in the calibration process.

Calibration refers to the process of minimizing measurement and output voltage errors by making small circuit adjustments. On the 611X E board, these adjustments take the form of writing values to onboard calibration DACs (CalDACs).

Some form of board calibration is required for all but the most forgiving applications. If you do not calibrate your board, your signals and measurements could have very large offset, gain, and linearity errors.

Three levels of calibration are available to you and described in this chapter. The first level is the fastest, easiest, and least accurate; whereas, the last level is the slowest, most difficult, and most accurate.

Loading Calibration Constants

The 611X E board is factory calibrated before shipment at approximately 25° C to the levels indicated in Appendix A, *Specifications*. The associated calibration constants—the values that were written to the CalDACs to achieve calibration in the factory—are stored in the onboard nonvolatile memory (EEPROM). Because the CalDACs have no memory capability, they do not retain calibration information when the board is unpowered. Loading calibration constants refers to the process of loading the CalDACs with the values stored in the EEPROM. NI-DAQ software determines when this is necessary and does it automatically. If you are not using NI-DAQ, you must load these values yourself.

In the EEPROM there is a user-modifiable calibration area in addition to the permanent factory calibration area. This means that you can load the CalDACs with values either from the original factory calibration or from a calibration that you subsequently performed.

This method of calibration is not very accurate because it does not take into account the fact that the board measurement and output voltage errors can vary with time and temperature. It is better to self-calibrate when the board is installed in the environment in which it will be used.

Self-Calibration

The 611X E board can measure and correct for almost all of its calibration-related errors without any external signal connections. Your National Instruments software provides a self-calibration method. This self-calibration process, which generally takes less than a minute, is the preferred method of assuring accuracy in your application. Initiate self-calibration to minimize the effects of any offset, gain, and linearity drifts, particularly those due to warmup.

Immediately after self-calibration, the only significant residual calibration error could be gain error due to time or temperature drift of the onboard voltage reference. This error is addressed by external calibration, which is discussed in the following section. If you are interested primarily in relative measurements, you can ignore a small amount of gain error, and self-calibration should be sufficient.

External Calibration

The 611X E board has an onboard calibration reference to ensure the accuracy of self-calibration. Its specifications are listed in [Appendix A, Specifications](#). The reference voltage is measured at the factory and stored in the EEPROM for subsequent self-calibrations. This voltage is stable enough for most applications, but if you are using your board at an extreme temperature or if the onboard reference has not been measured for a year or more, you may wish to externally calibrate your board.

An external calibration refers to calibrating your board with a known external reference rather than relying on the onboard reference. Redetermining the value of the onboard reference is part of this process and the results can be saved in the EEPROM, so you should not have to perform an external calibration very often. You can externally calibrate your board by calling the NI-DAQ calibration function.

To externally calibrate your board, be sure to use a very accurate external reference. The reference should be several times more accurate than the board itself. For example, to calibrate a 16-bit board, the external reference should be at least $\pm 0.001\%$ (± 10 ppm) accurate.

Specifications

This appendix lists the specifications of your 611X E board. These specifications are typical at 25° C unless otherwise noted.

PCI-6110E/6111E

Analog Input

Input Characteristics

Number of channels

PCI-6110E4 differential

PCI-6111E2 differential

Resolution.....12 bits, 1 in 4,096

Max sampling rate5 MS/s

Min sampling rate1 kS/s

Analog input characteristics

Input Range	Gain Error ¹	Offset Error	SFDR ²	CMRR ³	System Noise ⁴
±50 V	0.50%	10 mV	70 dB	32 dB	0.5
±20 V	0.50%	10 mV	70 dB	35 dB	0.5
±10 V	0.10%	0.8 mV	75 dB	50 dB	0.5
±5 V	0.05%	0.5 mV	75 dB	56 dB	0.5
±2 V	0.05%	0.28 mV	75 dB	62 dB	0.5
±1 V	0.05%	0.20 mV	75 dB	67 dB	0.5
±500 mV	0.05%	0.15 mV	75 dB	70 dB	0.6
±200 mV	0.05%	0.10 mV	75 dB	72 dB	1.0

¹Relative to reading, max

²All input ranges, DC to 100 kHz

³All input ranges, DC to 60 Hz

⁴LSB_{rms}, not including quantization

Input coupling	DC/AC
Max working voltage for all analog input channels	
+ input	Should remain within ± 11 V for ranges $\geq \pm 10$ V; should remain within ± 42 V for ranges $< \pm 10$ V
– input	Should remain within ± 11 V
Overvoltage protection	± 42 V
Inputs protected	
+ input	all channels
– input	all channels
FIFO buffer size	8,192 samples
Data transfers	DMA, interrupts, programmed I/O
DMA modes	Scatter-gather

Accuracy Information

See following table

PCI-6110E/6111E Accuracy Information

Nominal Range (V)	Absolute Accuracy						Relative Accuracy	
	% of Reading		Offset (mV)	Noise + Quantization (mV)		Temp Drift (%/°C)	Resolution (mV)	
	24 Hours	90 Days		1 Year	Single Pt.		Averaged	Theoretical
±50	0.51%	0.51%	35 mV	51 mV	4.4 mV	0.0005%	24 mV	5.8 mV
±20	0.51%	0.51%	20 mV	20 mV	1.8 mV	0.0005%	9.8 mV	2.3 mV
±10	0.11%	0.11%	5.7 mV	10 mV	0.88 mV	0.0005%	4.9 mV	1.2 mV
±5	0.057%	0.058%	3 mV	5.1 mV	0.44 mV	0.0005%	2.4 mV	0.58 mV
±2	0.057%	0.058%	1.3 mV	2 mV	0.18 mV	0.0005%	0.98 mV	0.23 mV
±1	0.057%	0.058%	0.7 mV	1 mV	0.088 mV	0.0005%	0.49 mV	0.12 mV
±0.5	0.057%	0.058%	0.4 mV	0.67 mV	0.059 mV	0.0005%	0.24 mV	0.077 mV
±0.2	0.057%	0.058%	0.2 mV	0.39 mV	0.035 mV	0.0005%	0.098 mV	0.046 mV

Note: Accuracies are valid for measurements following an internal E Series calibration. Averaged numbers assume dithering and averaging of 100 single-channel readings. Measurement accuracies are listed for operational temperatures within ±1° C of internal calibration temperature and ±10° C of external or factory calibration temperature. One year calibration interval recommended.

Transfer Characteristics

INL	± 0.5 LSB typ, ± 1 LSB max
DNL	± 0.3 LSB typ, ± 0.75 LSB max
Spurious free dynamic range (SFDR)	See table, analog input characteristics
Effective number of bits (ENOB)	11.0 bits, DC to 100 kHz
Offset error	See table, analog input characteristics

Amplifier Characteristics

Input impedance	1 M Ω in parallel with 100 pF
Input bias current	± 200 pA
Input offset current	± 100 pA
CMRR	See table, analog input characteristics

Dynamic Characteristics

Interchannel skew	1 ns typ $f_{in} = 100$ kHz input range = ± 10 V
Bandwidth (0.5 to -3 dB)	
Input range $> \pm 0.2$ V	5 MHz
Input range = ± 0.2 V	4 MHz
System noise	See table, analog input characteristics
Crosstalk	-80 dB, DC to 100 kHz

Stability

Recommended warm-up time	15 min.
Offset temperature coefficient	
Pregain	± 5 $\mu\text{V}/^\circ\text{C}$

Postgain	$\pm 50 \mu\text{V}/^\circ\text{C}$
Gain temperature coefficient.....	$\pm 20 \text{ ppm}/^\circ\text{C}$
Onboard calibration reference	
Level	5.000 V ($\pm 2.5 \text{ mV}$) (actual value stored in EEPROM)
Temperature coefficient	$\pm 0.6 \text{ ppm}/^\circ\text{C max}$
Long-term stability.....	$\pm 6 \text{ ppm}/\sqrt{1,000 \text{ h}}$

Analog Output

Output Characteristics

Number of channels	2 voltage
Resolution.....	16 bits, 1 in 65,536
Max update rate	
1 channel.....	4 MS/s, system dependent
2 channel.....	2.5 MS/s, system dependent
FIFO buffer size.....	2,048 samples
Data transfers.....	DMA, interrupts, programmed I/O
DMA modes	Scatter gather

Transfer Characteristics

Relative accuracy (INL).....	$\pm 4 \text{ LSB typ, } \pm 8 \text{ LSB max}$
DNL.....	$\pm 2 \text{ LSB typ, } \pm 8 \text{ LSB max}$
Offset error	$\pm 5.0 \text{ mV max}$
Gain error	
(relative to internal reference).....	$\pm 0.1\%$ of output range max

Voltage Output

Ranges	$\pm 10 \text{ V}$
Output coupling	DC

Output impedance	50 Ω \pm 5%
Current drive	\pm 5 mA min
Output stability	Any passive load
Protection	Short-circuit to ground
Power-on state.....	0 V

Dynamic Characteristics

Slew rate	300 V/ μ s
Noise	1 mV _{rms} , DC to 5 MHz
Spurious free dynamic range	75 dB, DC to 10 kHz

Stability

Offset temperature coefficient	\pm 500 μ V/ $^{\circ}$ C
Gain temperature coefficient	
Internal reference.....	\pm 50 ppm/ $^{\circ}$ C
External reference	\pm 25 ppm/ $^{\circ}$ C
Onboard calibration reference	
Level	5.000 V (\pm 2.5 mV) (actual value stored in EEPROM)
Temperature coefficient.....	\pm 0.6 ppm/ $^{\circ}$ C max
Long-term stability	\pm 6 ppm/ $\sqrt{1,000}$ h

Digital I/O

Number of channels	8 input/output
Compatibility	TTL/CMOS

Digital logic levels

Level	Min	Max
Input low voltage	0.0 V	0.8 V
Input high voltage	2.0 V	5.0 V
Input low current ($V_{in} = 0$ V)	—	-320 μ A
Input high current ($V_{in} = 5$ V)	—	10 μ A
Output low voltage ($I_{OL} = 24$ mA)	—	0.4 V
Output high voltage ($I_{OH} = 13$ mA)	4.35 V	—

Power-on stateInput (High-Z)

Data transfersProgrammed I/O

Timing I/O

Number of channels2 up/down counter/timers,
1 frequency scaler

Resolution

Counter/timers24 bits

Frequency scaler4 bits

CompatibilityTTL/CMOS

Base clocks available

Counter/timers20 MHz, 100 kHz

Frequency scaler10 MHz, 100 kHz

Base clock accuracy $\pm 0.01\%$

Max source frequency20 MHz

Min source pulse duration10 ns, edge-detect mode

Min gate pulse duration10 ns, edge-detect mode

Data transfers	DMA, interrupts, programmed I/O
DMA modes	Scatter-gather

Triggers

Analog Trigger

Source

PCI-6110E	All analog input channels, external trigger (PFI0/TRIG1)
PCI-6111E	All analog input channels, external trigger (PFI0/TRIG1)

Level \pm full-scale, internal;
 ± 10 V, external

Slope Positive or negative
(software selectable)

Resolution 8 bits, 1 in 256

Hysteresis Programmable

Bandwidth (-3 dB) 5 MHz internal/external

External input (PFI0/TRIG1)

Impedance	10 k Ω
Coupling	AC/DC
Protection	-0.5 V to ($V_{CC} + 0.5$) V when configured as a digital signal, ± 35 V when configured as an analog trigger signal or disabled, ± 35 V powered off

Digital Trigger

Compatibility TTL

Response Rising or falling edge

Pulse width..... 10 ns min

RTSI

Trigger Lines7

Bus Interface

TypeMaster, slave

Power Requirement

+5 VDC ($\pm 5\%$)

PCI-6110E2.5 A

PCI-6111E2.0 A

Power available at I/O connector+4.65 to +5.25 VDC at 1 A

Physical

Dimensions

(not including connectors)31.2 by 10.6 cm (12.3 by 4.2 in)

I/O connector68-pin male SCSI-II type

Environment

Operating temperature0° to 45° C

Storage temperature-20° to 70° C

Relative humidity5% to 90% noncondensing

Cable Connector Descriptions

The logo for Appendix B, featuring the word "Appendix" in a serif font above a large, bold, black letter "B". The entire logo is enclosed in a square border with a drop shadow effect.

Appendix
B

This appendix describes the cable connectors on your 611X E board.


Figure B-1 shows the pin assignments for the 68-pin 611X E connector. This connector is available when you use the SH6868EP cable assemblies with the 611X E board.

ACH0-	34	68	ACH0+
ACH1+	33	67	ACH0GND
ACH1GND	32	66	ACH1-
ACH2-1	31	65	ACH2+1
ACH3+1	30	64	ACH2GND ¹
ACH3GND ¹	29	63	ACH3-1
NC	28	62	NC
NC	27	61	NC
NC	26	60	NC
NC	25	59	NC
NC	24	58	NC
NC	23	57	NC
DAC0OUT	22	56	NC
DAC1OUT	21	55	AOGND
NC	20	54	AOGND
DIO4	19	53	DGND
DGND	18	52	DIO0
DIO1	17	51	DIO5
DIO6	16	50	DGND
DGND	15	49	DIO2
+5 V	14	48	DIO7
DGND	13	47	DIO3
DGND	12	46	SCANCLK
PFI0/TRIG1	11	45	EXTSTROBE*
PFI1/TRIG2	10	44	DGND
DGND	9	43	PFI2/CONVERT*
+5 V	8	42	PFI3/GPCTR1_SOURCE
DGND	7	41	PFI4/GPCTR1_GATE
PFI5/UPDATE*	6	40	GPCTR1_OUT
PFI6/WFTRIG	5	39	DGND
DGND	4	38	PFI7/STARTSCAN
PFI9/GPCTR0_GATE	3	37	PFI8/GPCTR0_SOURCE
GPCTR0_OUT	2	36	DGND
FREQ_OUT	1	35	DGND

1 NC on PCI-6111E

Figure B-1. 68-Pin 611XE Series Connector Pin Assignments

Common Questions

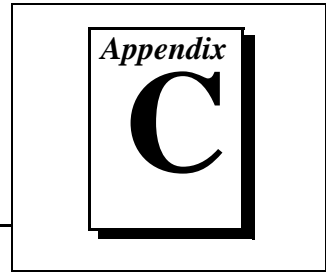

This appendix contains a list of commonly asked questions and their answers relating to usage and special features of your 611X E board.

General Information

What is the 611X E board?

The 611X E board is a switchless and jumperless enhanced MIO board that uses the DAQ-STC for timing.

What is the DAQ-STC?

The DAQ-STC is the system timing control application-specific integrated circuit (ASIC) designed by National Instruments and is the backbone of the 611X E board. The DAQ-STC contains seven 24-bit counters and three 16-bit counters. The counters are divided into the following three groups:

- Analog input—two 24-bit, two 16-bit counters
- Analog output—three 24-bit, one 16-bit counters
- General-purpose counter/timer functions—two 24-bit counters

The groups can be configured independently with timing resolutions of 50 ns or 10 μ s. With the DAQ-STC, you can interconnect a wide variety of internal timing signals to other internal blocks. The interconnection scheme is quite flexible and completely software configurable. New capabilities such as buffered pulse generation, equivalent time sampling, and seamlessly changing the sampling rate are possible.

What does sampling rate mean to me?

It means that this is the fastest you can acquire data on your board and still achieve accurate results. The 611X E board has a sampling rate of 5 MS/s. This sampling rate is at 5 MS/s regardless if 1 or 4 channels are acquiring data.

What type of 5 V protection does the 611X E board have?

The 611X E board has 5 V lines equipped with a self-resetting 1 A fuse.

Installation and Configuration

How do you set the base address for the 611X E board?

The base address of the 611X E board is assigned automatically through the PCI bus protocol. This assignment is completely transparent to you.

What jumpers should I be aware of when configuring my 611X E board?

The 611X E board is jumperless and switchless.

Which National Instruments document should I read first to get started using DAQ software?

Your NI-DAQ or application software release notes documentation is always the best starting place.

Analog Input and Output

I have connected a differential input signal, but my readings are random and drift rapidly. What's wrong?

Check your ground reference connections. Your signal may be referenced to a level that is considered *floating* with reference to the board ground reference. Even if you are in differential mode, the signal *must* still be referenced to the same ground level as the board reference. There are various methods of achieving this while maintaining a high common-mode rejection ratio (CMRR). These methods are outlined in [Chapter 4, Signal Connections](#).

I'm using the DACs to generate a waveform, but I discovered with a digital oscilloscope that there are glitches on the output signal. Is this normal?

When it switches from one voltage to another, any DAC produces glitches due to released charges. The largest glitches occur when the most significant bit (MSB) of the D/A code switches. You can build a lowpass deglitching filter to remove some of these glitches, depending on the frequency and nature of your output signal.

Can I synchronize a one-channel analog input data acquisition with a one-channel analog output waveform generation on my 611X E board?

Yes. One way to accomplish this is to use the waveform generation timing pulses to control the analog input data acquisition. To do this, follow steps 1 through 4 below, in addition to the usual steps for data acquisition and waveform generation configuration.

1. Enable the PFI5 line for output, as follows:
 - If you are using NI-DAQ, call `Select_Signal(deviceNumber, ND_PFI_5, ND_OUT_UPDATE, ND_HIGH_TO_LOW)`.
 - If you are using LabVIEW, invoke Route Signal VI with signal name set to PFI5 and signal source set to AO Update.
2. Set up data acquisition timing so that the timing signal for A/D conversion comes from PFI5, as follows:
 - If you are using NI-DAQ, call `Select_Signal(deviceNumber, ND_IN_CONVERT, ND_PFI_5, ND_HIGH_TO_LOW)`.
 - If you are using LabVIEW, invoke AI Clock Config VI with clock source code set to PFI pin, high to low, and clock source string set to 5.
3. Initiate analog input data acquisition, which will start only when the analog output waveform generation starts.
4. Initiate analog output waveform generation.

Timing and Digital I/O

What types of triggering can be hardware-implemented on my 611X E board?

Hardware digital and analog triggering are both supported on the 611X E board.

What added functionality does the DAQ-STC make possible in contrast to the Am9513?

The DAQ-STC incorporates much more than just 10 Am9513-style counters within one chip. In fact, the DAQ-STC has the complexity of more than 24 chips. The DAQ-STC makes possible PFI lines, analog triggering, selectable logic level, and frequency shift keying. The DAQ-STC also makes buffered operations possible, such as direct

up/down control, single or pulse train generation, equivalent time sampling, buffered period, and buffered semiperiod measurement.

What is the difference in timebases between the Am9513 counter/timer and the DAQ-STC?

The DAQ-STC-based MIO boards have a 20 MHz timebase. The Am9513-based MIO boards have a 1 MHz or 5 MHz timebase.

Will the counter/timer applications that I wrote previously, work with the DAQ-STC?

If you are using NI-DAQ with LabVIEW, some of your applications drawn using the CTR VIs will still run. However, there are many differences in the counters between the 611X E and other boards; the counter numbers are different, timebase selections are different, and the DAQ-STC counters are 24-bit counters (unlike the 16-bit counters on boards without the DAQ-STC).

If you are using the NI-DAQ language interface or LabWindows/CVI, the answer is no, the counter/timer applications that you wrote previously will not work with the DAQ-STC. You must use the GPCTR functions; ICTR and CTR functions will not work with the DAQ-STC. The GPCTR functions have the same capabilities as the ICTR and CTR functions, plus more, but you must rewrite the application with the GPCTR function calls.

I'm using one of the general-purpose counter/timers on my 611X E board, but I do not see the counter/timer output on the I/O connector. What am I doing wrong?

If you are using the NI-DAQ language interface or LabWindows/CVI, you must configure the output line to output the signal to the I/O connector. Use the `Select_Signal` call in NI-DAQ to configure the output line. By default, all timing I/O lines except EXTSTROBE* are tri-stated.

What are the PFIs and how do I configure these lines?

PFIs are Programmable Function Inputs. These lines serve as connections to virtually all internal timing signals.

If you are using the NI-DAQ language interface or LabWindows/CVI, use the `Select_Signal` function to route internal signals to the I/O

connector, route external signals to internal timing sources, or tie internal timing signals together.

If you are using NI-DAQ with LabVIEW and you want to connect external signal sources to the PFI lines, you can use AI Clock Config, AI Trigger Config, AO Clock Config, AO Trigger and Gate Config, CTR Mode Config, and CTR Pulse Config advanced level VIs to indicate which function the connected signal will serve. Use the Route Signal VI to enable the PFI lines to output internal signals.




Caution: *If you enable a PFI line for output, do not connect any external signal source to it; if you do, you can damage the board, the computer, and the connected equipment.*

What are the power-on states of the PFI and DIO lines on the I/O connector?

At system power-on and reset, both the PFI and DIO lines are set to high impedance by the hardware. This means that the board circuitry is not actively driving the output either high or low. However, these lines may have pull-up or pull-down resistors connected to them as shown in Table 4-2. These resistors weakly pull the output to either a logic high or logic low state. For example, DIO(0) will be in the high impedance state after power on, and Table 4-2 shows that there is a 50 k Ω pull-up resistor. This pull-up resistor will set the DIO(0) pin to a logic high when the output is in a high impedance state.

Customer Communication

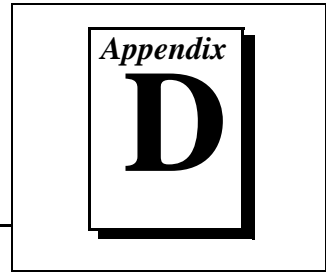

For your convenience, this appendix contains forms to help you gather the information necessary to help us solve your technical problems and a form you can use to comment on the product documentation. When you contact us, we need the information on the Technical Support Form and the configuration form, if your manual contains one, about your system configuration to answer your questions as quickly as possible.

National Instruments has technical assistance through electronic, fax, and telephone systems to quickly provide the information you need. Our electronic services include a bulletin board service, an FTP site, a fax-on-demand system, and e-mail support. If you have a hardware or software problem, first try the electronic support systems. If the information available on these systems does not answer your questions, we offer fax and telephone support through our technical support centers, which are staffed by applications engineers.

Electronic Services

Bulletin Board Support

National Instruments has BBS and FTP sites dedicated for 24-hour support with a collection of files and documents to answer most common customer questions. From these sites, you can also download the latest instrument drivers, updates, and example programs. For recorded instructions on how to use the bulletin board and FTP services and for BBS automated information, call 512 795 6990. You can access these services at:

United States: 512 794 5422

Up to 14,400 baud, 8 data bits, 1 stop bit, no parity

United Kingdom: 01635 551422

Up to 9,600 baud, 8 data bits, 1 stop bit, no parity

France: 01 48 65 15 59

Up to 9,600 baud, 8 data bits, 1 stop bit, no parity

FTP Support

To access our FTP site, log on to our Internet host, `ftp.natinst.com`, as anonymous and use your Internet address, such as `joesmith@anywhere.com`, as your password. The support files and documents are located in the `/support` directories.

Fax-on-Demand Support

Fax-on-Demand is a 24-hour information retrieval system containing a library of documents on a wide range of technical information. You can access Fax-on-Demand from a touch-tone telephone at 512 418 1111.

E-Mail Support (Currently USA Only)

You can submit technical support questions to the applications engineering team through e-mail at the Internet address listed below. Remember to include your name, address, and phone number so we can contact you with solutions and suggestions.

support@natinst.com

Telephone and Fax Support

National Instruments has branch offices all over the world. Use the list below to find the technical support number for your country. If there is no National Instruments office in your country, contact the source from which you purchased your software to obtain support.

Country	Telephone	Fax
Australia	03 9879 5166	03 9879 6277
Austria	0662 45 79 90 0	0662 45 79 90 19
Belgium	02 757 00 20	02 757 03 11
Brazil	011 288 3336	011 288 8528
Canada (Ontario)	905 785 0085	905 785 0086
Canada (Québec)	514 694 8521	514 694 4399
Denmark	45 76 26 00	45 76 26 02
Finland	09 725 725 11	09 725 725 55
France	01 48 14 24 24	01 48 14 24 14
Germany	089 741 31 30	089 714 60 35
Hong Kong	2645 3186	2686 8505
Israel	03 6120092	03 6120095
Italy	02 413091	02 41309215
Japan	03 5472 2970	03 5472 2977
Korea	02 596 7456	02 596 7455
Mexico	5 520 2635	5 520 3282
Netherlands	0348 433466	0348 430673
Norway	32 84 84 00	32 84 86 00
Singapore	2265886	2265887
Spain	91 640 0085	91 640 0533
Sweden	08 730 49 70	08 730 43 70
Switzerland	056 200 51 51	056 200 51 55
Taiwan	02 377 1200	02 737 4644
United Kingdom	01635 523545	01635 523154
United States	512 795 8248	512 794 5678

Technical Support Form

Photocopy this form and update it each time you make changes to your software or hardware, and use the completed copy of this form as a reference for your current configuration. Completing this form accurately before contacting National Instruments for technical support helps our applications engineers answer your questions more efficiently.

If you are using any National Instruments hardware or software products related to this problem, include the configuration forms from their user manuals. Include additional pages if necessary.

Name _____

Company _____

Address _____

Fax (____) _____ Phone (____) _____

Computer brand _____ Model _____ Processor _____

Operating system (include version number) _____

Clock speed _____ MHz RAM _____ MB Display adapter _____

Mouse ___yes ___no Other adapters installed _____

Hard disk capacity _____ MB Brand _____

Instruments used _____

National Instruments hardware product model _____ Revision _____

Configuration _____

National Instruments software product _____ Version _____

Configuration _____

The problem is: _____

List any error messages: _____

The following steps reproduce the problem: _____

PCI-6110E/6111E Hardware and Software Configuration Form

Record the settings and revisions of your hardware and software on the line to the right of each item. Complete a new copy of this form each time you revise your software or hardware configuration, and use this form as a reference for your current configuration. Completing this form accurately before contacting National Instruments for technical support helps our applications engineers answer your questions more efficiently.

National Instruments Products

PCI-6110E/6111E board _____

PCI-6110E/6111E board serial number _____

Base memory address of the PCI-6110E/6111E board _____

Interrupt level of the PCI-6110E/6111E board _____

National Instruments application software choice _____

Software version _____

Other Products

Computer make and model _____

Microprocessor _____

Clock frequency or speed _____

Type of video board installed _____

Operating system (DOS or Windows) _____

Operating system version _____

Operating system mode _____

Programming language _____

Programming language version _____

Other boards in system _____

Base memory address of other boards _____

Interrupt level of other boards _____

Documentation Comment Form

National Instruments encourages you to comment on the documentation supplied with our products. This information helps us provide quality products to meet your needs.

Title: *PCI-6110E/6111E User Manual*

Edition Date: April 1998

Part Number: 321759B-01

Please comment on the completeness, clarity, and organization of the manual.

If you find errors in the manual, please record the page numbers and describe the errors.

Thank you for your help.

Name _____

Title _____

Company _____

Address _____

Phone (____) _____ Fax (____) _____

Mail to: Technical Publications
National Instruments Corporation
6504 Bridge Point Parkway
Austin, TX 78730-5039

Fax to: Technical Publications
National Instruments Corporation
(512) 794-5678

Prefix	Meaning	Value
p-	pico-	10^{-12}
n-	nano-	10^{-9}
μ -	micro-	10^{-6}
m-	milli-	10^{-3}
k-	kilo-	10^3
M-	mega-	10^6
G-	giga-	10^9

Symbols/Numbers

°	degrees
>	greater than
≥	greater than or equal to
<	less than
≤	less than or equal to
/	per
%	percent
±	plus or minus
+	positive of, or plus

– negative of, or minus

Ω ohms

$\sqrt{\quad}$ square root of

+5 V +5 VDC source signal

A

A amperes

AC alternating current

ACH analog input channel signal

ACH0GND analog input channel ground signal

A/D analog-to-digital

ADC analog-to-digital converter—an electronic device, often an integrated circuit, that converts an analog voltage to a digital number

AI analog input

AIGATE analog input gate signal

AIGND analog input ground signal

ANSI American National Standards Institute

AO analog output

AOGND analog output ground signal

ASIC Application-Specific Integrated Circuit—a proprietary semiconductor component designed and manufactured to perform a set of specific functions.

B

bipolar a signal range that includes both positive and negative values (for example, –5 V to +5 V)

C

C	Celsius
CalDAC	calibration DAC
CH	channel—pin or wire lead to which you apply or from which you read the analog or digital signal. Analog signals can be single-ended or differential. For digital signals, you group channels to form ports. Ports usually consist of either four or eight digital channels
cm	centimeter
CMOS	complementary metal-oxide semiconductor
CMRR	common-mode rejection ratio—a measure of an instrument's ability to reject interference from a common-mode signal, usually expressed in decibels (dB)
CONVERT*	convert signal
counter/timer	a circuit that counts external pulses or clock pulses (timing)
CTR	counter

D

D/A	digital-to-analog
DAC	digital-to-analog converter—an electronic device, often an integrated circuit, that converts a digital number into a corresponding analog voltage or current
DAC0OUT	analog channel 0 output signal
DAC1OUT	analog channel 1 output signal
DAQ	data acquisition—a system that uses the computer to collect, receive, and generate electrical signals
DAQ-STC	Data acquisition system timing controller. An application-specific integrated circuit (ASIC) for the system timing requirements of a

general A/D and D/A system, such as a system containing the National Instruments E Series boards.

dB	decibel—the unit for expressing a logarithmic measure of the ratio of two signal levels: $dB=20\log_{10} V_1/V_2$, for signals in volts
DC	direct current
DGND	digital ground signal
DI	digital input
DIFF	differential mode
DIO	digital input/output
DIP	dual inline package
dithering	the addition of Gaussian noise to an analog input signal
DMA	direct memory access—a method by which data can be transferred to/from computer memory from/to a device or memory on the bus while the processor does something else. DMA is the fastest method of transferring data to/from computer memory.
DNL	differential nonlinearity—a measure in least significant bit of the worst-case deviation of code widths from their ideal value of 1 LSB
DO	digital output
E	
EEPROM	electrically erasable programmable read-only memory—ROM that can be erased with an electrical signal and reprogrammed
EXTSTROBE	external strobe signal
F	
FIFO	first-in first-out memory buffer—FIFOs are often used on DAQ devices to temporarily store incoming or outgoing data until that data can be read or written. For example, an analog input FIFO stores the results of A/D conversions until the data can be read into

system memory. Programming the DMA controller and servicing interrupts can take several milliseconds in some cases. During this time, data accumulates in the FIFO for future retrieval. With a larger FIFO, longer latencies can be tolerated. In the case of analog output, a FIFO permits faster update rates, because the waveform data can be stored in the FIFO ahead of time. This again reduces the effect of latencies associated with getting the data from system memory to the DAQ device.

FREQ_OUT frequency output signal

ft feet

G

GATE gate signal

GPCTR general-purpose counter signal

GPCTR0_GATE general-purpose counter 0 gate signal

GPCTR0_OUT general-purpose counter 0 output signal

GPCTR0_SOURCE general-purpose counter 0 clock source signal

GPCTR0_UP_DOWN general-purpose counter 0 up down signal

GPCTR1_GATE general-purpose counter 1 gate signal

GPCTR1_OUT general-purpose counter 1 output signal

GPCTR1_SOURCE general-purpose counter 1 clock source signal

GPCTR1_UP_DOWN general-purpose counter 1 up down signal

H

h hour

hex hexadecimal

Hz hertz

I

INL	integral nonlinearity—For an ADC, deviation of codes of the actual transfer function from a straight line.
I/O	input/output—the transfer of data to/from a computer system involving communications channels, operator interface devices, and/or data acquisition and control interfaces
I_{OH}	current, output high
I_{OL}	current, output low

K

kHz	kilohertz
-----	-----------

L

LED	light emitting diode
LSB	least significant bit

M

m	meter
MB	megabytes of memory
MHz	megahertz
MIO	multifunction I/O
MITE	MXI Interface to Everything
MSB	most significant bit
mux	multiplexer—a switching device with multiple inputs that sequentially connects each of its inputs to its output, typically at high speeds, in order to measure several signals with a single analog input channel

mV millivolts

N

NC normally closed, or not connected

NI-DAQ National Instruments driver software for DAQ hardware

noise an undesirable electrical signal—Noise comes from external sources such as the AC power line, motors, generators, transformers, fluorescent lights, CRT displays, computers, electrical storms, welders, radio transmitters, and internal sources such as semiconductors, resistors, and capacitors. Noise corrupts signals you are trying to send or receive.

NRSE nonreferenced single-ended mode—all measurements are made with respect to a common (NRSE) measurement system reference, but the voltage at this reference can vary with respect to the measurement system ground

O

OUT output pin—a counter output pin where the counter can generate various TTL pulse waveforms

P

PCI Peripheral Component Interconnect—a high-performance expansion bus architecture originally developed by Intel to replace ISA and EISA. It is achieving widespread acceptance as a standard for PCs and work-stations; it offers a theoretical maximum transfer rate of 132 MB/s.

PFI Programmable Function Input

PFI0/TRIG1 PFI0/trigger 1

PFI1/TRIG2 PFI1/trigger 2

PFI2/CONVERT* PFI2/convert

PFI3/GPCTR1_SOURCE PFI3/general purpose counter 1 source

PFI4/GPCTR1_GATE	PFI4/general-purpose counter 1 gate
PFI5/UPDATE*	PFI5/update
PFI6/WFTRIG	PFI6/waveform trigger
PFI7/STARTSCAN	PFI7/start of scan
PFI8/GPCTR0_SOURCE	PFI8/general-purpose counter 0 source
PFI9/GPCTR0_GATE	PFI9/general-purpose counter 0 gate
PGIA	Programmable Gain Instrumentation Amplifier
port	(1) a communications connection on a computer or a remote controller (2) a digital port, consisting of four or eight lines of digital input and/or output
ppm	parts per million
pu	pull-up
R	
RAM	random access memory
rms	root mean square
RSE	referenced single-ended mode—all measurements are made with respect to a common reference measurement system or a ground. Also called a grounded measurement system
RTD	resistive temperature detector—a metallic probe that measures temperature based upon its coefficient of resistivity
RTSibus	real-time system integration bus—the National Instruments timing bus that connects DAQ boards directly, by means of connectors on top of the boards, for precise timing synchronization between multiple boards
RTSI_OSC	RTSI Oscillator—RTSI bus master clock

S

s	seconds
S	samples
SCANCLK	scan clock signal
SCXI	Signal Conditioning eXtensions for Instrumentation—the National Instruments product line for conditioning low-level signals within an external chassis near sensors so only high-level signals are sent to DAQ boards in the noisy computer environment
SE	single-ended—a term used to describe an analog input that is measured with respect to a common ground
settling time	the amount of time required for a voltage to reach its final value within specified limits
signal conditioning	the manipulation of signals to prepare them for digitizing
SISOURCE	SI counter clock signal
SOURCE	source signal
S/s	samples per second—used to express the rate at which a DAQ board samples an analog signal
STARTSCAN	start scan signal
system noise	a measure of the amount of noise seen by an analog circuit or an ADC when the analog inputs are grounded

T

TC	terminal count—the ending value of a counter
t_{gh}	gate hold time
t_{gsu}	gate setup time
t_{gw}	gate pulse width
t_{out}	output delay time

THD	total harmonic distortion—the ratio of the total rms signal due to harmonic distortion to the overall rms signal, in decibel or a percentage
thermocouple	a temperature sensor created by joining two dissimilar metals. The junction produces a small voltage as a function of the temperature.
TRIG	trigger signal
t_{sc}	source clock period
t_{sp}	source pulse width
TTL	transistor-transistor logic
U	
UI	update interval
UISOURCE	update interval counter clock signal
unipolar	a signal range that is always positive (for example, 0 to +10 V)
UPDATE	update signal
V	
V	volts
VDC	volts direct current
VI	virtual instrument—(1) a combination of hardware and/or software elements, typically used with a PC, that has the functionality of a classic stand-alone instrument (2) a LabVIEW software module (VI), which consists of a front panel user interface and a block diagram program
V_{IH}	volts, input high
V_{IL}	volts, input low
V_{in}	volts in
V_m	measured voltage

V_{OH}	volts, output high
V_{OL}	volts, output low
V_{ref}	reference voltage
V_{rms}	volts, root mean square

W

WFTRIG	waveform generation trigger signal
--------	------------------------------------

Numbers

+5 V signal

- description (table), 4-3
- power connections, 4-15
- self-resetting fuse, 4-15, C-2

A

AC input coupling, 3-4

ACH<0..3>+ signal

- analog input connections, 4-8
- description (table), 4-3
- differential connections
 - ground-referenced signal sources (figure), 4-11
 - nonreferenced or floating signal sources (figure), 4-12
- signal summary (table), 4-6

ACH<0..3>- signal

- analog input connections, 4-8
- description (table), 4-3
- differential connections
 - ground-referenced signal sources (figure), 4-11
 - nonreferenced or floating signal sources (figure), 4-12
- signal summary (table), 4-6

ACH<0..3>GND signal

- description (table), 4-3
- differential connections
 - ground-referenced signal sources (figure), 4-11

- nonreferenced or floating signal sources (figure), 4-12

- signal summary (table), 4-6

AIGATE signal, 4-25

- amplifier characteristic specifications, A-3 to A-4

analog input, 3-2 to 3-5

- dither, 3-4 to 3-5
- input coupling, 3-4
- input mode, 3-2 to 3-3
- input polarity and range, 3-3 to 3-4
- questions about, C-2 to C-3
- selection considerations, 3-4
- signal connections, 4-8
- specifications, A-1 to A-5

- amplifier characteristics, A-3 to A-4

- dynamic characteristics, A-4

- input characteristics, A-1 to A-2

- stability, A-4 to A-5

- transfer characteristics, A-2 to A-3

analog output, 3-5

- questions about, C-2 to C-3
- signal connections, 4-13
- specifications, A-5 to A-6
 - dynamic characteristics, A-6
 - output characteristics, A-5
 - stability, A-6
 - transfer characteristics, A-5
 - voltage output, A-5 to A-6

analog trigger

- above-high-level analog triggering mode (figure), 3-8
- avoiding false triggering (note), 3-6

- below-low-level analog triggering mode (figure), 3-7
- block diagrams
 - PCI-6110E, 3-6
 - PCI-6111E, 3-7
- high-hysteresis analog triggering mode (figure), 3-9
- inside-region analog triggering mode (figure), 3-8
- low-hysteresis analog triggering mode (figure), 3-9
- specifications, A-8
- AOGND signal
 - analog output signal connections, 4-13
 - description (table), 4-3
 - signal summary (table), 4-6

B

- bipolar input, 3-3
- block diagrams
 - PCI-6110E, 3-1
 - PCI-6111E, 3-2
- board configuration, 2-2
- bulletin board support, D-1
- bus interface specifications, A-9

C

- cables. *See also* I/O connectors.
 - custom cabling, 1-5 to 1-6
 - field wiring considerations, 4-35 to 4-36
 - optional equipment, 1-5
- calibration, 5-1 to 5-3
 - external calibration, 5-2 to 5-3
 - loading calibration constants, 5-1 to 5-2
 - self-calibration, 5-2
- clocks, board and RTSI, 3-12
- commonly asked questions. *See* questions and answers.
- common-mode signal rejection, 4-12

- ComponentWorks software, 1-3
- configuration
 - PCI-6110E/6111E, 2-2
 - questions about, C-2
- connectors. *See* I/O connectors.
- CONVERT* signal
 - input timing (figure), 4-24
 - multiplexer for controlling (figure), 3-11
 - output timing (figure), 4-24
 - signal routing, 3-11 to 12
 - timing connections, 4-23 to 4-25
- counter/timer applications, C-4 to C-5
- customer communication, *xiv*, D-1 to D-2

D

- DAC0OUT signal
 - analog output signal connections, 4-13
 - description (table), 4-3
 - signal summary (table), 4-6
- DAC1OUT signal
 - analog output signal connections, 4-13
 - description (table), 4-3
 - signal summary (table), 4-6
- DAQ timing connections, 4-17 to 4-26
 - AIGATE signal, 4-25
 - CONVERT* signal, 4-23 to 4-25
 - EXTSTROBE* signal, 4-18 to 4-19
 - SCANCLK signal, 4-18
 - SISOURCE signal, 4-25 to 4-26
 - STARTSCAN signal, 4-22 to 4-23
 - TRIG1 signal, 4-19 to 4-20
 - TRIG2 signal, 4-20 to 4-21
 - typical posttriggered acquisition (figure), 4-17
 - typical pretriggered acquisition (figure), 4-18
- DAQ-STC system timing controller
 - overview, 1-1
 - questions about, C-1, C-3 to C-4

data acquisition timing connections. *See* DAQ timing connections.

DC input coupling, 3-4

DGND signal

description (table), 4-3

digital I/O connections, 4-13 to 4-14

signal summary (table), 4-6

timing connections, 4-16

differential measurements, 4-9 to 4-12

common-mode signal rejection, 4-12

connection considerations, 4-10

DIFF input mode, 3-2 to 3-3

floating signal sources, 4-9, 4-11 to 4-12

ground-referenced signal sources,
4-9, 4-11

nonreferenced signal sources,
4-11 to 4-12

recommended configuration (table), 4-10

digital I/O

operation, 3-10

questions about, C-3 to C-5

signal connections, 4-13 to 4-14

specifications, A-6 to A-7

digital trigger specifications, A-8

DIO<0..7> signal

description (table), 4-3

digital I/O connections, 4-13 to 4-14

signal summary (table), 4-6

dither

enabling, 3-4 to 3-5

signal acquisition effects (figure), 3-5

documentation

conventions used in manual, *xii-xiii*

National Instruments documentation,
xiii-xiv

organization of manual, *xi-xii*

related documentation, *xiv*

dynamic characteristic specifications

analog input, A-4

analog output, A-6

E

EEPROM storage of calibration constants, 5-1

electronic support services, D-1 to D-2

e-mail support, D-2

environment specifications, A-9

environmental noise, avoiding, 4-35 to 4-36

equipment, optional, 1-5

EXTSTROBE* signal

description (table), 4-3

signal summary (table), 4-6

timing connections, 4-18 to 4-19

F

fax and telephone support numbers, D-2

Fax-on-Demand support, D-2

field wiring considerations, 4-35 to 4-36

floating signal sources

description, 4-9

differential connections, 4-11 to 4-12

recommended configuration (table), 4-10

FREQ_OUT signal

description (table), 4-5

general-purpose timing connections, 4-35

signal summary (table), 4-7

frequently asked questions. *See* questions and answers.

FTP support, D-1

fuse, self-resetting, 4-15, C-2

G

general-purpose timing signal connections,
4-29 to 4-35

FREQ_OUT signal, 4-35

GPCTR0_GATE signal, 4-30 to 4-31

GPCTR0_OUT signal, 4-31

GPCTR0_SOURCE signal, 4-29 to 4-30

GPCTR0_UP_DOWN signal, 4-31

GPCTR1_GATE signal, 4-32 to 4-33

GPCTR1_OUT signal, 4-33

GPCTR1_SOURCE signal, 4-32
 GPCTR1_UP_DOWN signal,
 4-34 to 4-35
 questions about, C-4 to C-5
 glitches, C-2
 GPCTR0_GATE signal, 4-30 to 4-31
 GPCTR0_OUT signal
 description (table), 4-5
 general-purpose timing connections, 4-31
 signal summary (table), 4-7
 GPCTR0_SOURCE signal, 4-29 to 4-30
 GPCTR0_UP_DOWN signal, 4-31
 GPCTR1_GATE signal, 4-32 to 4-33
 GPCTR1_OUT signal
 description (table), 4-4
 general-purpose timing connections, 4-33
 signal summary (table), 4-7
 GPCTR1_SOURCE signal, 4-32
 GPCTR1_UP_DOWN signal, 4-34 to 4-35
 ground-referenced signal sources
 description, 4-9
 differential connections, 4-11
 recommended configuration (table), 4-10

H

hardware installation
 procedure, 2-1 to 2-2
 unpacking PCI-6110E/6111E, 1-6
 hardware overview
 analog input, 3-2 to 3-5
 dither, 3-4 to 3-5
 input mode, 3-2 to 3-3
 input polarity and range, 3-3 to 3-4
 selection considerations, 3-4
 analog output, 3-5
 analog trigger, 3-6 to 3-9
 block diagrams
 PCI-6110E, 3-1
 PCI-6111E, 3-2
 digital I/O, 3-10

timing signal routing, 3-11 to 13
 board and RTSI clocks, 3-12
 CONVERT* signal routing
 (figure), 3-11
 programmable function inputs, 3-12
 RTSI triggers, 3-13

I

input characteristic specifications, A-1 to A-2
 input mode. *See* differential measurements.
 input polarity and range, 3-3 to 3-4
 actual range and measurement precision
 (table), 3-3
 selection considerations, 3-4
 installation
 hardware, 2-1 to 2-2
 questions about, C-2
 software, 2-1
 unpacking PCI-6110E/6111E, 1-6
 I/O connectors, 4-1 to 4-7
 cable connectors for
 PCI-6110E/6111E, 1-6
 exceeding maximum ratings
 (warning), 4-1
 I/O signal summary (table), 4-6 to 4-7
 pin assignments (figure), 4-2, B-2
 signal descriptions (table), 4-3 to 4-5

L

LabVIEW and LabWindows/CVI application
 software, 1-2 to 1-3

M

manual. *See* documentation.

N

NI-DAQ driver software, 1-3 to 1-4
 noise, avoiding, 4-35 to 4-36
 NRSE (nonreferenced single-ended input),
 4-11 to 4-12

O

optional equipment, 1-5
 output characteristic specifications, A-5

P

PCI-6110E/6111E. *See also* hardware overview.
 custom cabling, 1-5 to 1-6
 optional equipment, 1-5
 overview, 1-1 to 1-2
 questions about, C-1 to C-5
 analog input and output, C-2 to C-3
 general information, C-1 to C-2
 installation and configuration, C-2
 timing and digital I/O, C-3 to C-5
 requirements for getting started, 1-2
 software programming choices, 1-2 to 1-4
 ComponentWorks, 1-3
 LabVIEW and LabWindows/CVI application software, 1-2 to 1-3
 National Instruments application software, 1-2 to 1-3
 NI-DAQ driver software, 1-3 to 1-4
 register-level programming, 1-4
 VirtualBench, 1-3
 unpacking, 1-6
 PFI0/TRIG1 signal
 description (table), 4-4
 signal summary (table), 4-6
 PFI1/TRIG2 signal
 description (table), 4-4
 signal summary (table), 4-6

PFI2/CONVERT* signal
 description (table), 4-4
 signal summary (table), 4-6
 PFI3/GPCTR1_SOURCE signal
 description (table), 4-4
 signal summary (table), 4-6
 PFI4/GPCTR1_GATE signal
 description (table), 4-4
 signal summary (table), 4-7
 PFI5/UPDATE* signal
 description (table), 4-4
 signal summary (table), 4-7
 PFI6/WFTRIG signal
 description (table), 4-5
 signal summary (table), 4-7
 PFI7/STARTSCAN signal
 description (table), 4-5
 signal summary (table), 4-7
 PFI8/GPCTR0_SOURCE signal
 description (table), 4-5
 signal summary (table), 4-7
 PFI9/GPCTR0_GATE signal
 description (table), 4-5
 signal summary (table), 4-7
 PFIs (programmable function inputs),
 4-16 to 4-17
 connecting to external signal source (warning), C-5
 overview, 4-16 to 4-17
 questions about, C-4 to C-5
 signal routing, 3-12
 timing input connections, 4-16 to 4-17
 PGIA (programmable gain instrumentation amplifier)
 analog input connections, 4-8
 common-mode signal rejection, 4-12
 differential connections
 floating signal sources (figure), 4-12
 ground-referenced signal sources, 4-11
 physical specifications, A-9

pin assignments (figure), 4-2, B-2
 polarity selection, analog input, 3-3 to 3-4
 posttriggered data acquisition, 4-17
 power connections

- +5 V power pins, 4-15
- self-resetting fuse, 4-15

 power requirement specifications, A-9
 pretriggered data acquisition, 4-17 to 4-18
 programmable function inputs (PFIs). *See* PFIs (programmable function inputs).
 programmable gain instrumentation amplifier. *See* PGIA (programmable gain instrumentation amplifier).

Q

questions and answers

- analog input and output, C-2 to C-3
- general information, C-1 to C-2
- installation and configuration, C-2
- timing and digital I/O, C-3 to C-5

R

register-level programming, 1-4
 requirements for getting started, 1-2
 RTSI clocks, 3-12
 RTSI trigger lines, 3-13

- signal connection (figure), 3-13
- specifications, A-8

S

SCANCLK signal

- description (table), 4-3
- signal summary (table), 4-6
- timing connections, 4-18

 signal connections

- analog input, 4-8
- analog output, 4-13
- differential measurements, 4-9 to 4-12

common-mode signal rejection, 4-12
 connection considerations, 4-10
 floating signal sources, 4-9, 4-11 to 4-12
 ground-referenced signal sources, 4-9, 4-11
 nonreferenced signal sources, 4-11 to 4-12
 recommended configuration (table), 4-10
 digital I/O, 4-13 to 4-14
 field wiring considerations, 4-35 to 4-36
 I/O connector, 4-1 to 4-7

- exceeding maximum ratings (warning), 4-1
- I/O signal summary (table), 4-6 to 4-7
- pin assignments (figure), 4-2, B-2
- signal descriptions (table), 4-3 to 4-5

 power connections, 4-15
 RTSI trigger lines, 3-13
 timing connections, 4-15 to 4-35

- DAQ timing connections, 4-17 to 4-26
 - AIGATE signal, 4-25
 - CONVERT* signal, 4-23 to 4-25
 - EXTSTROBE* signal, 4-18 to 4-19
 - SCANCLK signal, 4-18
 - SISOURCE signal, 4-25 to 4-26
 - STARTSCAN signal, 4-22 to 4-23
 - TRIG1 signal, 4-19 to 4-20
 - TRIG2 signal, 4-20 to 4-21
- typical posttriggered acquisition (figure), 4-17
- typical pretriggered acquisition (figure), 4-18

general-purpose timing signal
 connections, 4-29 to 4-35
 FREQ_OUT signal, 4-35
 GPCTR0_GATE signal,
 4-30 to 4-31
 GPCTR0_OUT signal, 4-31
 GPCTR0_SOURCE signal,
 4-29 to 4-30
 GPCTR0_UP_DOWN
 signal, 4-31
 GPCTR1_GATE signal,
 4-32 to 4-33
 GPCTR1_OUT signal, 4-33
 GPCTR1_SOURCE signal, 4-32
 GPCTR1_UP_DOWN signal,
 4-34 to 4-35
 programmable function input
 connections, 4-16 to 4-17
 waveform generation timing
 connections, 4-26 to 4-29
 UISOURCE signal, 4-28 to 4-29
 UPDATE* signal, 4-27 to 4-28
 WFTRIG signal, 4-26 to 4-27
 types of signal sources, 4-9
 floating, 4-9
 ground-referenced, 4-9
 SISOURCE signal, 4-25 to 4-26
 software installation, 2-1
 software programming choices, 1-2 to 1-4
 ComponentWorks, 1-3
 LabVIEW and LabWindows/CVI
 application software, 1-2 to 1-3
 National Instruments application
 software, 1-2 to 1-3
 NI-DAQ driver software, 1-3 to 1-4
 register-level programming, 1-4
 VirtualBench, 1-3
 specifications
 analog input, A-1 to A-5
 amplifier characteristics, A-3 to A-4
 dynamic characteristics, A-4

 input characteristics, A-1 to A-2
 stability, A-4 to A-5
 transfer characteristics, A-2 to A-3
 analog output, A-5 to A-6
 dynamic characteristics, A-6
 output characteristics, A-5
 stability, A-6
 transfer characteristics, A-5
 voltage output, A-5 to A-6
 analog trigger, A-8
 bus interface, A-9
 digital I/O, A-6 to A-7
 digital trigger, A-8
 environment, A-9
 physical, A-9
 power requirements, A-9
 RTSI, A-8
 timing I/O, A-7 to A-8
 stability specifications
 analog input, A-4 to A-5
 analog output, A-6
 STARTSCAN signal
 input timing (figure), 4-22
 output timing (figure), 4-23
 timing connections, 4-22 to 4-23

T

technical support, D-1 to D-2
 telephone and fax support numbers, D-2
 theory of operation. *See* hardware overview.
 timing connections, 4-15 to 4-35
 DAQ timing connections, 4-17 to 4-26
 AIGATE signal, 4-25
 CONVERT* signal, 4-23 to 4-25
 EXTSTROBE* signal, 4-18 to 4-19
 SCANCLK signal, 4-18
 SISOURCE signal, 4-25 to 4-26
 STARTSCAN signal, 4-22 to 4-23
 TRIG1 signal, 4-19 to 4-20
 TRIG2 signal, 4-20 to 4-21

- typical posttriggered acquisition (figure), 4-17
- typical pretriggered acquisition (figure), 4-18
- general-purpose timing signal
 - connections, 4-29 to 4-35
 - FREQ_OUT signal, 4-35
 - GPCTR0_GATE signal, 4-30 to 4-31
 - GPCTR0_OUT signal, 4-31
 - GPCTR0_SOURCE signal, 4-29 to 4-30
 - GPCTR0_UP_DOWN signal, 4-31
 - GPCTR1_GATE signal, 4-32 to 4-33
 - GPCTR1_OUT signal, 4-33
 - GPCTR1_SOURCE signal, 4-32
 - GPCTR1_UP_DOWN signal, 4-34 to 4-35
- programmable function input
 - connections, 4-16 to 4-17
- questions about, C-3 to C-5
- timing I/O connections (figure), 4-16
- waveform generation timing connections, 4-26 to 4-29
 - UISOURCE signal, 4-28 to 4-29
 - UPDATE* signal, 4-27 to 4-28
 - WFTRIG signal, 4-26 to 4-27
- timing I/O specifications, A-7 to A-8
- timing signal routing, 3-11 to 3-13
 - board and RTSI clocks, 3-12
 - CONVERT* signal routing (figure), 3-11
 - programmable function inputs, 3-12
 - RTSI triggers, 3-13
- transfer characteristic specifications
 - analog input, A-2 to A-3
 - analog output, A-5
- TRIG1 signal
 - input timing (figure), 4-20
 - output timing (figure), 4-20
 - timing connections, 4-19 to 4-20
- TRIG2 signal
 - input timing (figure), 4-21
 - output timing (figure), 4-21
 - timing connections, 4-20 to 4-21
- trigger, analog
 - above-high-level analog triggering mode (figure), 3-8
 - avoiding false triggering (note), 3-6
 - below-low-level analog triggering mode (figure), 3-7
 - block diagrams
 - PCI-6110E, 3-6
 - PCI-6111E, 3-7
 - high-hysteresis analog triggering mode (figure), 3-9
 - inside-region analog triggering mode (figure), 3-8
 - low-hysteresis analog triggering mode (figure), 3-9
 - specifications, A-8
- triggers
 - questions about, C-3
 - specifications
 - analog trigger, A-8
 - digital trigger, A-8

U

- UISOURCE signal, 4-28 to 4-29
- unpacking PCI-6110E/6111E, 1-6
- UPDATE* signal
 - input signal timing (figure), 4-28
 - output signal timing (figure), 4-28
 - timing connections, 4-27 to 4-28

V

- VCC signal (table), 4-6
- VirtualBench software, 1-3
- voltage output specifications, A-5 to A-6

W

waveform generation, questions about, C-3

waveform generation timing connections,
4-26 to 4-29

UISOURCE signal, 4-28 to 4-29

UPDATE* signal, 4-27 to 4-28

WFTRIG signal, 4-26 to 4-27

WFTRIG signal

input signal timing (figure), 4-27

output signal timing (figure), 4-27

timing connections, 4-26 to 4-27

wiring considerations, 4-35 to 4-36

Free Manuals Download Website

<http://myh66.com>

<http://usermanuals.us>

<http://www.somanuals.com>

<http://www.4manuals.cc>

<http://www.manual-lib.com>

<http://www.404manual.com>

<http://www.luxmanual.com>

<http://aubethermostatmanual.com>

Golf course search by state

<http://golfingnear.com>

Email search by domain

<http://emailbydomain.com>

Auto manuals search

<http://auto.somanuals.com>

TV manuals search

<http://tv.somanuals.com>