




OPERATING INSTRUCTIONS

HH804U

DUAL INPUT RTD THERMOMETER

1 YEAR
WARRANTY

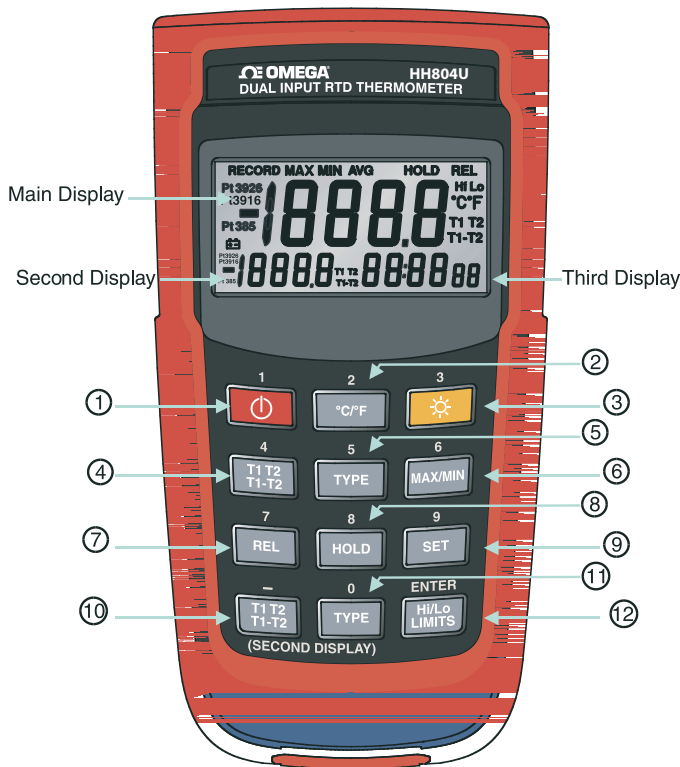

MADE IN TAIWAN

INTRODUCTION

This instrument is a 4_ digit, compact-sized portable digital thermometer designed to use external 100_ Platinum RTD as temperature sensor. Temperature indication follows Reference Temperature/Resistance Tables (Pt385 for European Curve, Alpha=.00385. Pt3926 for American Curve, Alpha=.003926. Pt3916 for Japan Curve, Alpha=.003916.)

SAFETY INFORMATION

It is recommended that you read the safety and operation instructions before using the thermometer.

WARNING

To avoid electrical shock, do not use this instrument when working voltages at the measurement surface over 24V AC or DC.

WARNING

To avoid damage or burns, do not take temperature measurements in microwave ovens.

ENVIRONMENTAL

Ambient Operating Ranges:

0°C to 50°C (32°F to 122°F) <70% R.H.

Storage Temperature:

-20°C to 60°C (-4°F to 140°F) <80% R.H.

GENERAL

Display:

4_ digit liquid crystal display (LCD) with maximum reading of 19999

Overload: "----.-" or "OL" is display.

Battery:

1.5V x 4 PCS (SIZE AAA) R03P.

Battery Life:

200 hours typical with carbon zinc battery

Auto power off: 30 minutes

Dimensions:

160mm(H) x83mm(W) x 38mm(D)

Weight: Approx. 255g including batteries.

SPECIFICATIONS

ELECTRICAL

Temperature Scale: Celsius or Fahrenheit user-selectable

Measurement Range:

Pt385(100_) -200°C to 800°C, (-328°F to 1472°F)

Pt3916/Pt3926(100_) -200°C to 630°C, (-328°F to 1166°F)

Resolution: 0.1°C or 0.2°F

Accuracy:

Accuracy is specified for operating temperatures over the range of 18°C to 28°C (64°F to 82°F), for 1 year, not including RTD probe error.

±(0.05% rdg + 0.2°C) on °C scale

±(0.05% rdg + 0.4°F) on °F scale

Temperature Coefficient:

0.1 times the applicable accuracy specification per °C from 0°C to 18°C and 28°C to 50°C (32°F to 64°F and 82°F to 122°F).

Input Protection:

24V dc or 24V ac rms maximum input voltage on any combination of input pins.

Maximum Differential Common Mode Voltage (Maximum Voltage between T1 and T2 during measurement): 1volt.

Reading Rate: 1sample/second.

Input Connector:

Accepts 4 pin mini-DIN connectors.

Download from www.Somanuals.com. All Manuals Search And Download.

OPERATING INSTRUCTIONS

1. Power Button

The button turns the thermometer on or off. In the SET mode the unit cannot be powered off. Exit the SET mode to power off.

APO function mode

Press "" power button for more than 6 seconds to disable auto power function. The display will show "APO OFF".

2. °C/°F Selecting the Temperature Scale (Main display)

Readings are displayed in either degrees Celsius(°C) or degrees Fahrenheit(°F). When the thermometer is turned on, it is set to the temperature scale that was in use when the thermometer was last turned off. To change the temperature scale, press the °C/°F key.

3. " " Display Back-Light

Press the "" key to turn on or turn off the back light.

4. T1 T2/T1-T2 Main display Input Selection

The input selection button determines which input is shown on the display; T1 ,T2 or the difference between the two probes (T1-T2). When thermometer is turned on, it is set to T1.

5. TYPE(Pt385/Pt3926/Pt3916) Input RTD Probe Select (Main display)

The TYPE button selects the RTD curve to use for the input currently shown. When the thermometer is turned on, it is set to the curve that selected when the thermometer was last turned off.

6. MIN MAX with Time record Mode (only Main display)

Press MIN MAX key to enter the MIN MAX Recording mode, (displays Maximum reading with time, Minimum reading with time and Average reading stored in recording mode). In the this mode the automatic power-off feature is disabled and key, °C/°F key, REL key, SET key, Hi/Lo Li key and main display T1 T2 T1- T2 key, TYPE key are disabled. beeper emits a tone when a new minimum or maximum value is recorded. Push MIN MAX key to cycle through the MAX, MIN and AVG readings. If an overload is recorded, the averaging function is Stopped. In the mode, press HOLD key to stop the recording of readings, all values are zen, press again to restart recording. To prevent accidental loss of MAX and AVG data, in this mode can only be cancelled by pressing hold down the MIN MAX key for 2 seconds to exit and erased recorded readings.

7. REL Relative mode (only Main display)

Press REL key to enter the Relative mode, zero the display, and store displayed Reading as a reference value and annunciator REL is displayed. Press REL key again to exit the relative mode. The relative value can be entered by the user. (See "SET mode" later in this manual.) When the sired Relative value has been entered, press REL key to enter the Relative mode, press SET key use set Relative value as a reference value. Press key again to exit the relative mode. In the Relative mode, the value (can >±1999.9 counts) shown on the LCD is always the difference between stored reference and the present reading.

8. HOLD Mode (only Main display)

Press the HOLD key to enter the Data Hold mode, the "HOLD" annunciator is displayed. When HOLD mode is selected, the thermometer held the sent readings and stops all further measurements. Press the HOLD again to cancel HOLD mode causing thermometer to resume taking urents. In the MIN/MAX recording mode, press HOLD key to stop the cording. Press HOLD key again to resume recording. (Previously recorded read are not erased).

9. SET mode (Relative value set, Time set and Hi/Lo Limits value set)

9.1 Press SET key to enter Relative values SET mode (Press ENTER key escape relative values set mode), REL set mode. = = = = is displayed main display. Relative value is entered via overlay numbers, then

Time set mode. (Press ENTER key can escape Time set mode) =, =, =, = : = is displayed in second and third display. Time (hours, minutes, seconds) value is entered via overlay numbers, then press overlay ENTER key. Time start from set time value, enter Hi/Lo Limits value set mode.

Hi Limit value set mode, (Press ENTER key can escape Hi Limit value set mode), =, =, =, = is displayed in main display, Hi Limit value is entered via overlay numbers, then press overlay ENTER key, stored the Hi Limit value, enter Lo Limit value set mode (Press ENTER key can escape Lo Limit value set mode), =, =, =, = is displayed in main display, Lo Limit value is entered via overlay numbers, then press overlay ENTER key, stored the Lo Limit value and exit SET mode.

When the thermometer is turned on. The Relative set value and Hi/Lo Limits set value that was in use when thermometer was last turned off set values.

T1/T2 T1-T2 second display Input Selection

The input selection button determines which input is shown on the second display; T1, T2 or the difference between the two probes (T1-T2). When the thermometer is turned on, it is set to T2.

TYPE(Pt385/Pt3926/Pt3916) Input RTD Probe select (second display)



The TYPE button selects the RTD curve to use for the input currently shown. When the thermometer is turned on, it is set to the curve that was selected when the thermometer was last turned off.

Hi/Lo Limits mode (only Main display)

Press the Hi/Lo Limits button to enter the Hi/Lo Limits comparative mode, when the input temperature exceeds the Hi or Lo Limits value, the beeper emits a continuous pulse tone. Press the Hi/Lo Limits button again to exit Hi/Lo Limits mode.

RTD PROBE CONNECTION

P/N: 14061-0800-9
MINI DIN PLUG



TEMPERATURE VS RESISTANCE TABLE(ITS90)

°C	Pt385	Pt3926	Pt3916
-200°C	18.521	16.996	17.057
-100°C	60.256	59.479	59.565
0°C	100.000	100.000	100.000
100°C	138.505	139.272	139.171
200°C	175.856	177.362	177.155
300°C	212.052	214.275	213.957
400°C	247.092	250.018	249.584
500°C	280.977	284.591	284.036
600°C	313.708	317.994	317.313
700°C	345.280	-	-
800°C	375.700	-	-

The policy of OMEGA Engineering, Inc. to comply with all worldwide safety and EMC/EMI regulations that apply. OMEGA is constantly pursuing certification of its products to the latest European New Approach Directives. OMEGA will add the CE mark to every appropriate device certification.

Information contained in this document is believed to be correct, but OMEGA accepts no liability for any errors it contains, and reserves the right to alter specifications without notice. **WARNING:** These products are not designed for use in, and should not be used for, human applications.

WARNING

To avoid possible electrical shock, disconnect the thermocouple connectors from the thermometer before removing the cover.

Battery Replacement

- Power is supplied by 4pcs 1.5V (SIZE AAA) R03P.
- The "E" appears on the LCD display when replacement is needed. To replace battery remove screw from back of meter and lift off the battery cover.
- Remove the battery from battery contacts and replace.
- When not in use for long periods the batteries should be removed.
- Do not store in locations with high temperatures, or high humidity.

Cleaning

Periodically wipe the case with a damp cloth and detergent, do not use abrasives or solvents.



OMEGAnet® On-Line Service
omega.com

Internet e-mail
info@omega.com

Servicing North America:

U.S.A.: ISO 9001 Certified
One Omega Drive, Box 4047
Stamford, CT 06907-0047
Tel: (203) 359-1660
FAX: (203) 359-7700
e-mail: info@omega.com

Canada:
976 Bergar
Laval (Quebec) H7L 5A1, Canada
Tel: (514) 856-6928
FAX: (514) 856-6886
e-mail: info@omega.ca

For immediate technical or application assistance:

U.S.A. and Canada:
Sales Service: 1-800-826-6342 / 1-800-TC-OMEGA®
Customer Service: 1-800-622-2378 / 1-800-622-BEST®
Engineering Service: 1-800-872-9436 / 1-800-USA-WHEN®
Mexico:
En Español: (001) 203-359-7803
FAX: (001) 203-359-7807
e-mail: espanol@omega.com
info@omega.com.mx

Servicing Europe:

Czech Republic:
Fryštatska 184, 733 01 Karvina, Czech Republic
Tel: +420 (0)59 6311899
FAX: +420 (0)59 6311114
Toll Free: 0800-1-66342
e-mail: info@omegashop.cz

United Kingdom
ISO 9002 Certified
One Omega Drive
River Bend Technology Centre
Northbank, Irlam
Manchester M44 5BD

Germany/Austria:
Daimlerstrasse 26, D-75392
Deckenpfronn, Germany
Tel: +49 (0)7056 9398-0
FAX: +49 (0)7056 9398-29
Toll Free in Germany: 0800 639 7678
e-mail: info@omega.de

United Kingdom
Tel: +44 (0)161 777 6611
FAX: +44 (0)161 777 6622
Toll Free in United Kingdom:
0800-488-488
e-mail: sales@omega.co.uk

RETURN REQUESTS/INQUIRIES

Direct all warranty and repair requests/inquiries to the OMEGA Customer Service Department. BEFORE RETURNING ANY PRODUCT(S) TO OMEGA, PURCHASER MUST OBTAIN AN AUTHORIZED RETURN (AR) NUMBER FROM OMEGA'S CUSTOMER SERVICE DEPARTMENT (IN ORDER TO AVOID PROCESSING DELAYS). The assigned AR number should then be marked on the outside of the return package and on any correspondence.

The purchaser is responsible for shipping charges, freight, insurance and proper packaging to prevent breakage in transit.

FOR **WARRANTY** RETURNS, please have the following information available BEFORE contacting OMEGA:

- Purchase Order number under which the product was PURCHASED,
- Model and serial number of the product under warranty, and
- Repair instructions and/or specific problems relative to the product.

FOR **NON-WARRANTY** REPAIRS, consult OMEGA for current repair charges. Have the following information available BEFORE contacting OMEGA:

- Purchase Order number to cover the COST of the repair,
- Model and serial number of the product, and
- Repair instructions and/or specific problems relative to the product.

OMEGA's policy is to make running changes, not model changes, whenever an improvement is possible. This affords our customers the latest in technology and engineering.

OMEGA is a registered trademark of OMEGA ENGINEERING, INC.

© Copyright 2007 OMEGA ENGINEERING, INC. All rights reserved. This document may not be copied, photocopied, reproduced, translated, or reduced to any electronic medium or machine-readable form, in whole or in part, without the prior written consent of OMEGA ENGINEERING, INC.

WARRANTY/DISCLAIMER

OMEGA ENGINEERING, INC. warrants this unit to be free of defects in materials and workmanship for a period of **13 months** from date of purchase. OMEGA's WARRANTY adds an additional one (1) month grace period to the normal **one (1) year product warranty** to cover handling and shipping time. This ensures that OMEGA's customers receive maximum coverage on each product.

If the unit malfunctions, it must be returned to the factory for evaluation. OMEGA's Customer Service Department will issue an Authorized Return (AR) number immediately upon phone or written request. Upon examination by OMEGA, if the unit is found to be defective, it will be repaired or replaced at no charge. OMEGA's WARRANTY does not apply to defects resulting from any action of the purchaser, including but not limited to mishandling, improper interfacing, operation outside of design limits, improper repair, or unauthorized modification. This WARRANTY is VOID if the unit shows evidence of having been tampered with or shows evidence of having been damaged as a result of excessive corrosion; or current, heat, moisture or vibration; improper specification; misapplication; misuse or other operating conditions outside of OMEGA's control. Components in which wear is not warranted, include but are not limited to contact points, fuses, and triacs.

OMEGA is pleased to offer suggestions on the use of its various products. However, OMEGA neither assumes responsibility for any omissions or errors nor assumes liability for any damages that result from the use of its products in accordance with information provided by OMEGA, either verbal or written. OMEGA warrants only that the parts manufactured by the company will be as specified and free of defects. OMEGA MAKES NO OTHER WARRANTIES OR REPRESENTATIONS OF ANY KIND WHATSOEVER, EXPRESSED OR IMPLIED, EXCEPT THAT OF TITLE, AND ALL IMPLIED WARRANTIES INCLUDING ANY WARRANTY OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE ARE HEREBY DISCLAIMED. LIMITATION OF LIABILITY: The remedies of purchaser set forth herein are exclusive, and the total liability of OMEGA with respect to this order, whether based on contract, warranty, negligence, indemnification, strict liability or otherwise, shall not exceed the purchase price of the component upon which liability is based. In no event shall OMEGA be liable for consequential, incidental or special damages.

CONDITIONS: Equipment sold by OMEGA is not intended to be used, nor shall it be used: (1) as a "Basic Component" under 10 CFR 21 (NRC), used in or with any nuclear installation or activity; or (2) in medical applications or used on humans. Should any Product(s) be used in or with any nuclear installation or activity, medical application, used on humans, or misused in any way, OMEGA assumes no responsibility as set forth in our basic WARRANTY/DISCLAIMER language, and, additionally, purchaser will indemnify OMEGA and hold OMEGA harmless from any liability or damage whatsoever arising out of the use of the Product(s) in such a manner.

Where Do I Find Everything I Need for
Process Measurement and Control?
OMEGA...Of Course!
Shop online at omega.com

TEMPERATURE

- Thermocouple, RTD & Thermistor Probes, Connectors, Panels & Assemblies
- Wire: Thermocouple, RTD & Thermistor
- Calibrators & Ice Point References
- Recorders, Controllers & Process Monitors
- Infrared Pyrometers

PRESSURE, STRAIN AND FORCE

- Transducers & Strain Gages
- Load Cells & Pressure Gages
- Displacement Transducers
- Instrumentation & Accessories

FLOW/LEVEL

- Rotameters, Gas Mass Flowmeters & Flow Computers
- Air Velocity Indicators
- Turbine/Paddlewheel Systems
- Totalizers & Batch Controllers

pH/CONDUCTIVITY

- pH Electrodes, Testers & Accessories
- Benchtop/Laboratory Meters
- Controllers, Calibrators, Simulators & Pumps
- Industrial pH & Conductivity Equipment

DATA ACQUISITION

- Data Acquisition & Engineering Software
- Communications-Based Acquisition Systems
- Plug-in Cards for Apple, IBM & Compatibles
- Datalogging Systems
- Recorders, Printers & Plotters

HEATERS

- Heating Cable
- Cartridge & Strip Heaters
- Immersion & Band Heaters
- Flexible Heaters
- Laboratory Heaters

ENVIRONMENTAL MONITORING AND CONTROL

- Metering & Control Instrumentation
- Refractometers
- Pumps & Tubing
- Air, Soil & Water Monitors
- Industrial Water & Wastewater Treatment
- pH, Conductivity & Dissolved Oxygen Instruments

Free Manuals Download Website

<http://myh66.com>

<http://usermanuals.us>

<http://www.somanuals.com>

<http://www.4manuals.cc>

<http://www.manual-lib.com>

<http://www.404manual.com>

<http://www.luxmanual.com>

<http://aubethermostatmanual.com>

Golf course search by state

<http://golfingnear.com>

Email search by domain

<http://emailbydomain.com>

Auto manuals search

<http://auto.somanuals.com>

TV manuals search

<http://tv.somanuals.com>